

Note d'application

25mer Oligonucleotide Purification (0.5 μ mole scale)

Waters Corporation




This is an Application Brief and does not contain a detailed Experimental section.

Abstract

This application brief highlights the oligonucleotide purification using XTerra C₁₈ columns.

Introduction

25mer oligonucleotide has been analyzed in this application brief.

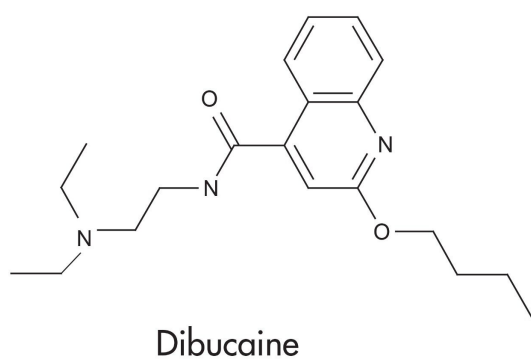

Experimental

HPLC Method


Column:	XTerra MS C ₁₈ 4.6 x 50 mm, 2.5 μm (p/n: 186000602)
Mobile phase A:	5% ACN, 95% 100 mM Triethylammonium acetate, pH 7.0
Mobile phase B:	30% ACN, 70% 100 mM Triethylammonium acetate, pH 7.0
Flow rate:	1.0 mL/min

Injection volume:	80 μ L
Temperature:	60°C
Detection:	UV @ 260 nm
Instrument:	Alliance 2695, 2996 PDA

Gradient

Time (min)	%A	%B
0	80	20
15	42.5	57.5

Results and Discussion

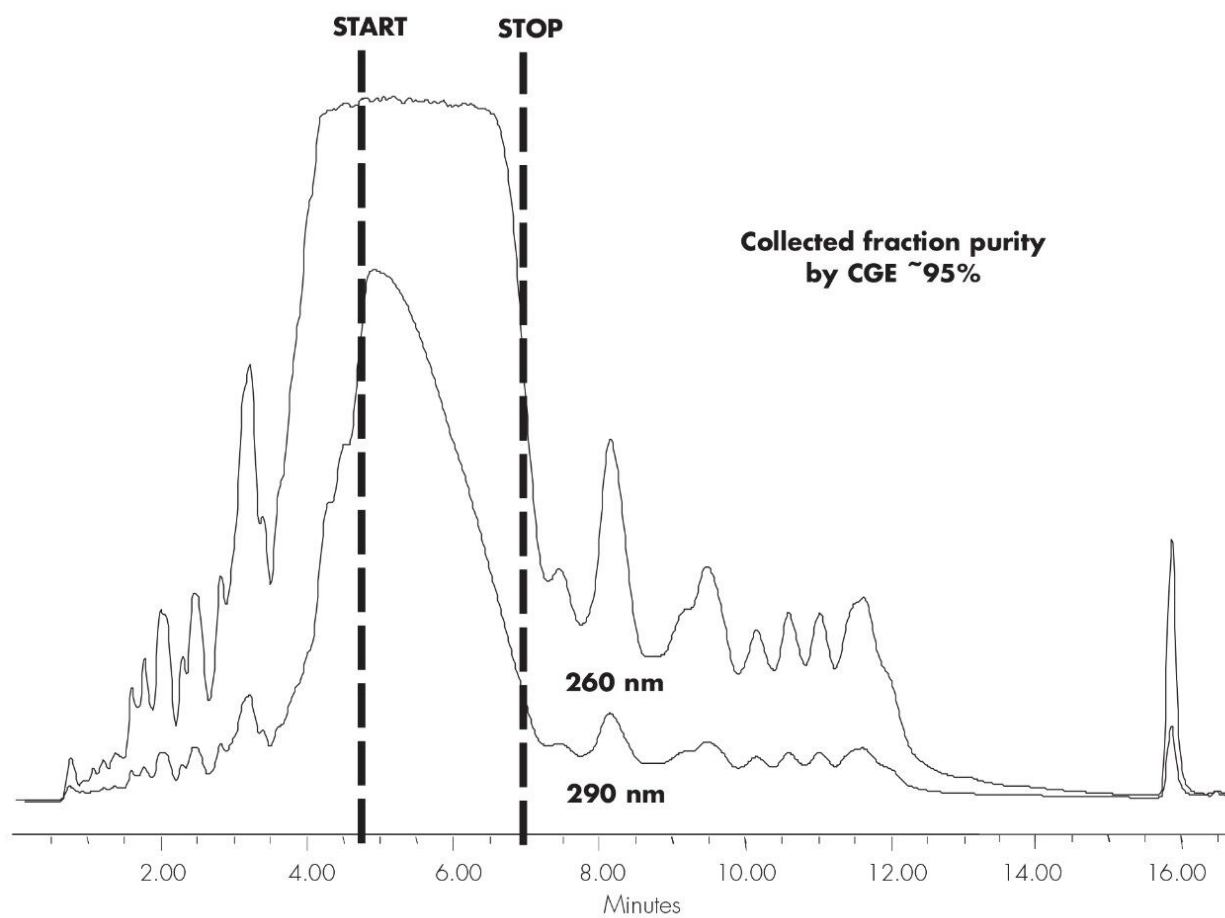

Featured Products

Alliance HPLC <<https://www.waters.com/514248>>

WA20738.002, June 2002

