
## Waters™

# Cytochrome C Tryptic Digest – pH 10.0, XTerra RP<sub>18</sub>

Waters Corporation

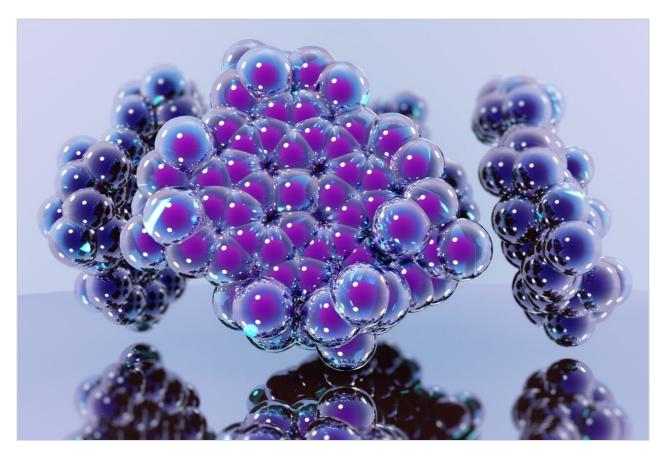

This is an Application Brief and does not contain a detailed Experimental section.

Abstract

This application brief highlights the analysis of cytochrome C using XTerra RP<sub>18</sub> columns.

1				- 1					
ı	nt	۱r	$\cap$	М	1.1	0	ŤΙ	$\cap$	n
н	111	u	U	u	u	$\cup$	UΙ	U	ш

Cytochrome C has been studied in this application brief.

## Experimental

#### **HPLC Conditions**

Column: XTerra RP $_{18}$  4.6 x 50 mm, 3.5  $\mu$ m (p/n:

186000434)

Mobile phase A: H<sub>2</sub>O

Mobile phase B: ACN

Mobile phase C: 100 mM HCOOH, pH 10.0

Flow rate: 0.75 mL/min, 0.2 mL/min to MS

Injection volume: 50  $\mu$ L (25  $\mu$ g)

Temperature: Ambient

Detection: MS ESI+

Instrument: Alliance 2790, Micromass Quattro Ultima


#### Gradient

Time	Profile					
(min)	%A	%B	%C			
0.0	90	0	10			
45.0	50	40	10			
45.0	10	80	10			
50.0	10	80	10			

#### **MS** Conditions

MS sytem: Micromass ZQ Ion source: ESI+ 3.5 kV Capillary: Cone: 30 V Extractor: 3.0 150 °C Source temp.: 400 °C Desolvation temp.: Cone gas flow: 60 L/hr Desolvation gas flow: 550 L/hr

### Results and Discussion

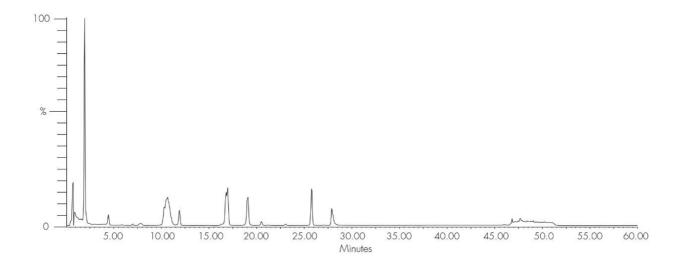

## Featured Products

Alliance HPLC <a href="https://www.waters.com/514248">https://www.waters.com/514248</a>

WA20738.030, June 2002

© 2021 Waters Corporation. All Rights Reserved.