


Note d'application

Oxybutynin in Rat Plasma

Waters Corporation

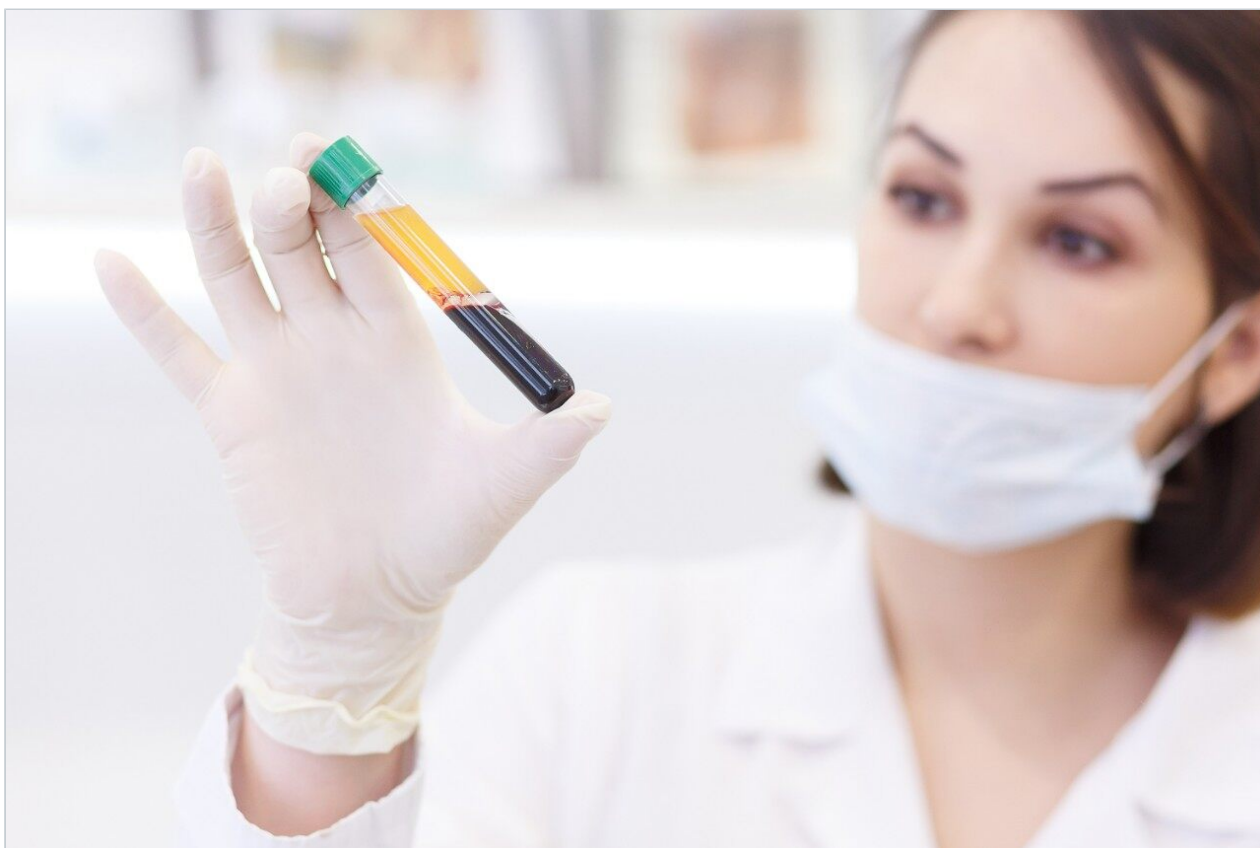


This is an Application Brief and does not contain a detailed Experimental section.

Abstract

This application brief highlights the analysis of oxybutynin using XTerra MS C₁₈ columns.

Introduction

Oxybutynin in rat plasma has been studied in this application brief.

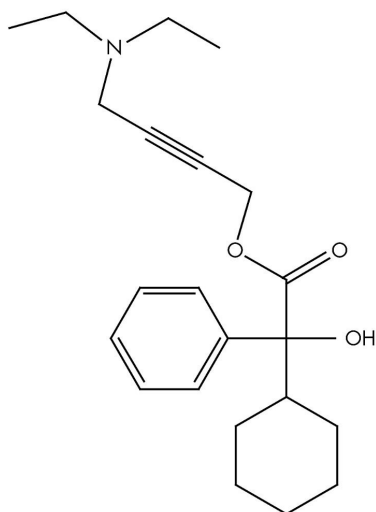

Oxybutynin

Experimental

HPLC Conditions


Column:	XTerra MS C ₁₈ 2.1 x 30 mm, 3.5 μm (p/n: 186000398)
Mobile phase A:	1.0% NH ₄ OH
Mobile phase B:	ACN
Isocratic mobile phase composition:	45% A; 55% B

Flow rate:	0.2 mL/min
Injection volume:	30 µL
Detection:	MS ESI+
Instrument:	Alliance 2790, Micromass Quattro Ultima

MS Conditions


Ion source:	ESI+
Source temp.:	150 °C
Gas cell:	1.5e ⁻³ mbar, 25 eV
Desolvation temp.:	350 °C
Cone gas flow:	150 L/hr
Drying gas flow:	600 L/hr
Cone voltage:	30 V

Oasis® MCX Extraction Method
Oasis® MCX Extraction Plate, 10 mg/96 well
Part Number 186000259

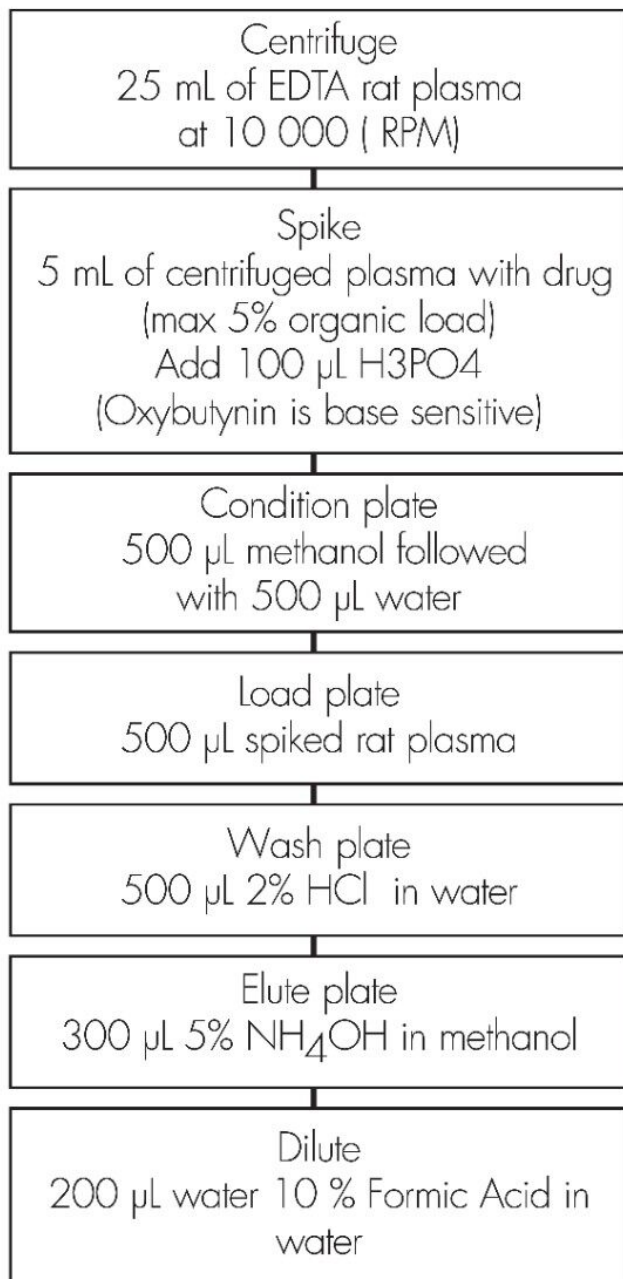

Results and Discussion

CID mass spectra

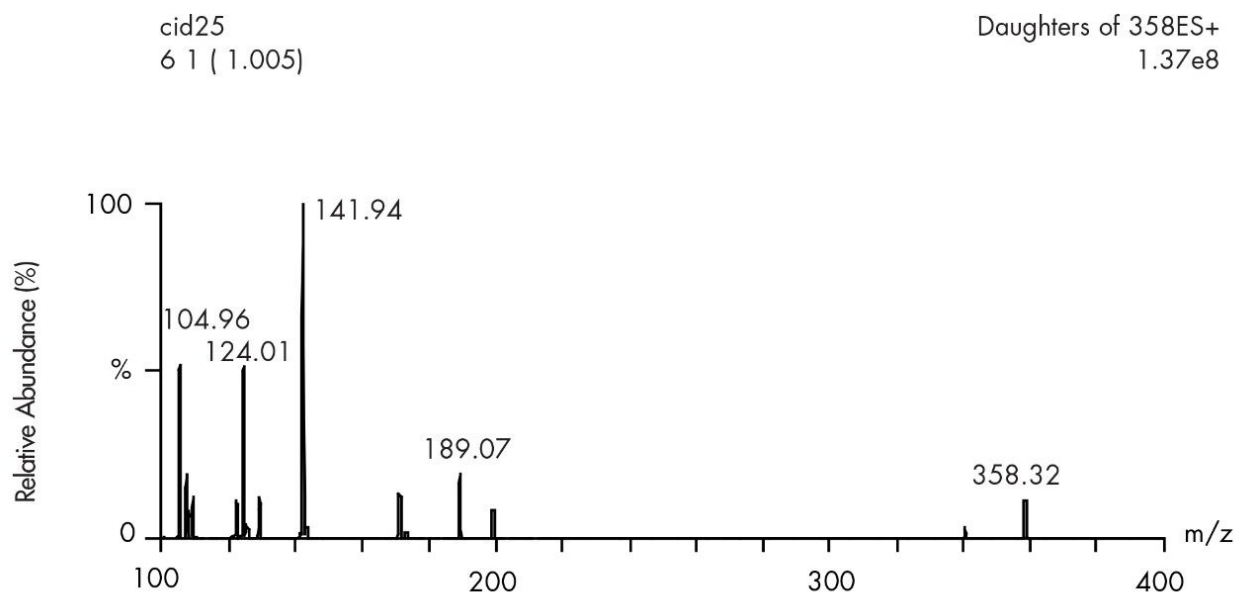

Featured Products

Alliance HPLC <<https://www.waters.com/514248>>

WA20738.083, June 2002