


Note d'application

Ranitidine in Serum

Waters Corporation

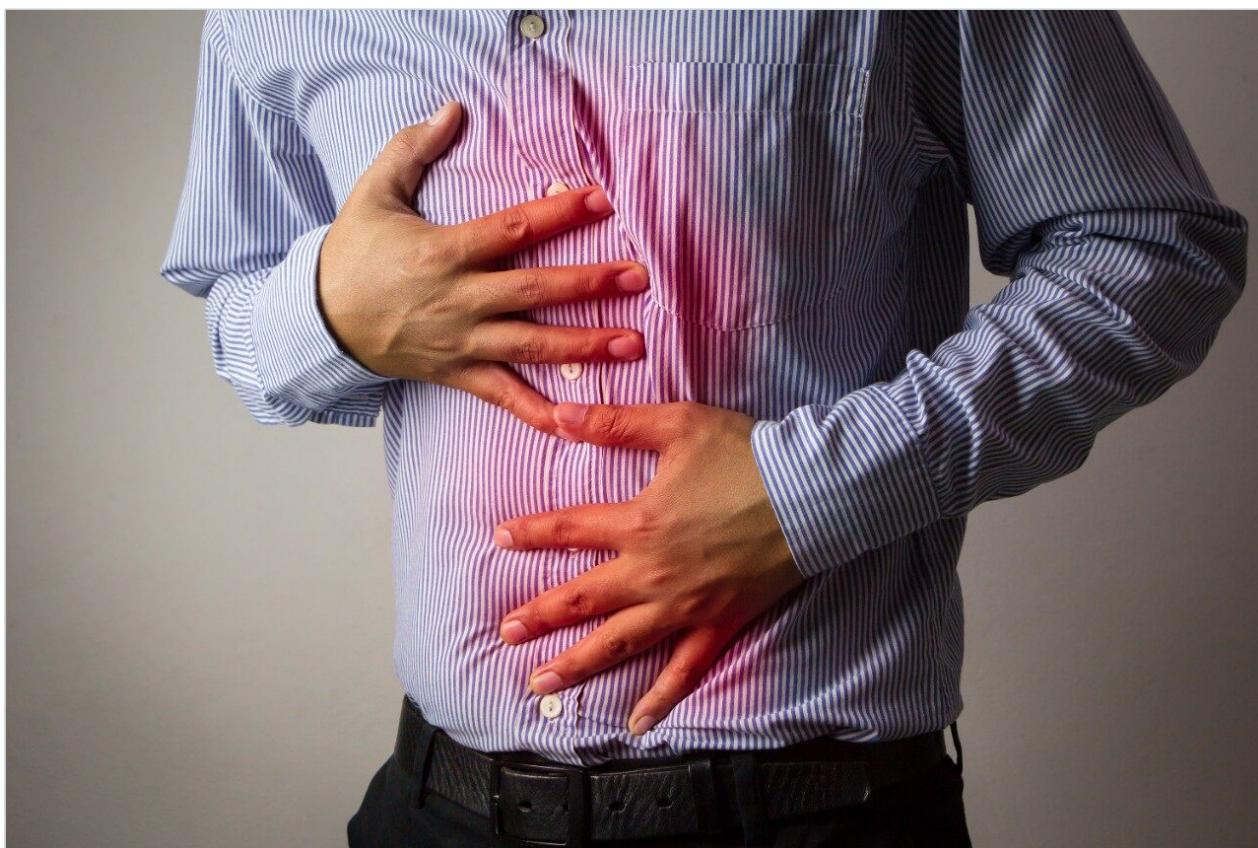

This is an Application Brief and does not contain a detailed Experimental section.


Abstract

This application brief highlights the analysis of ranitidine in serum using Symmetry Shield RP₈ Columns.


Introduction

The compounds analyzed in this study are:

1. Sulfanilamide (I.S.)
2. Ranitidine

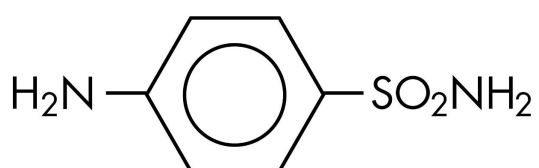

1. Sulfanilamide

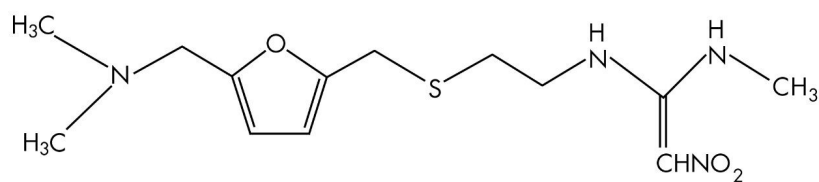

2. Ranitidine

Experimental

HPLC Method


Column:	Symmetry Shield RP ₈ , 3.9 x 150 mm, 5 μm
Guard column:	Symmetry guard column, 3.9 x 20 mm, 5 μm
Part numbers:	Column - WAT200655, Guard - WAT200675

Mobile phase:	20 mM potassium phosphate, pH 3.0/methanol 97:3
Flow rate:	1.0 mL/min
Injection volume:	50 µL of reconstituted porcine serum extract
Temperature:	30° C
Detection:	UV @ 220 nm

Oasis® HLB Extraction Method


Oasis® HLB 1 cc/30mg Extraction Cartridge

Part Number WAT094225

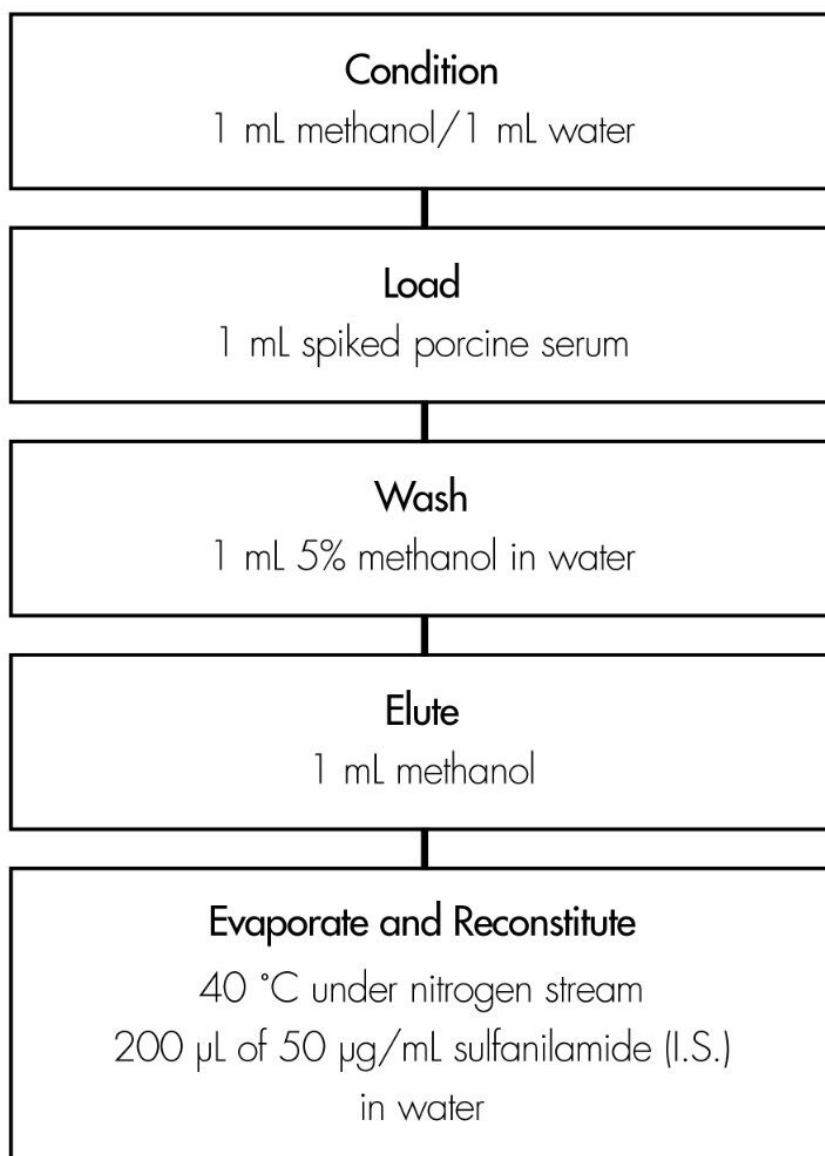

Results and Discussion

Compound	Concentration $\mu\text{g/mL}$	% Recovery	%RSD (n=6)
Ranitidine	0.100	104%	1.9%
	0.500	102%	1.7%

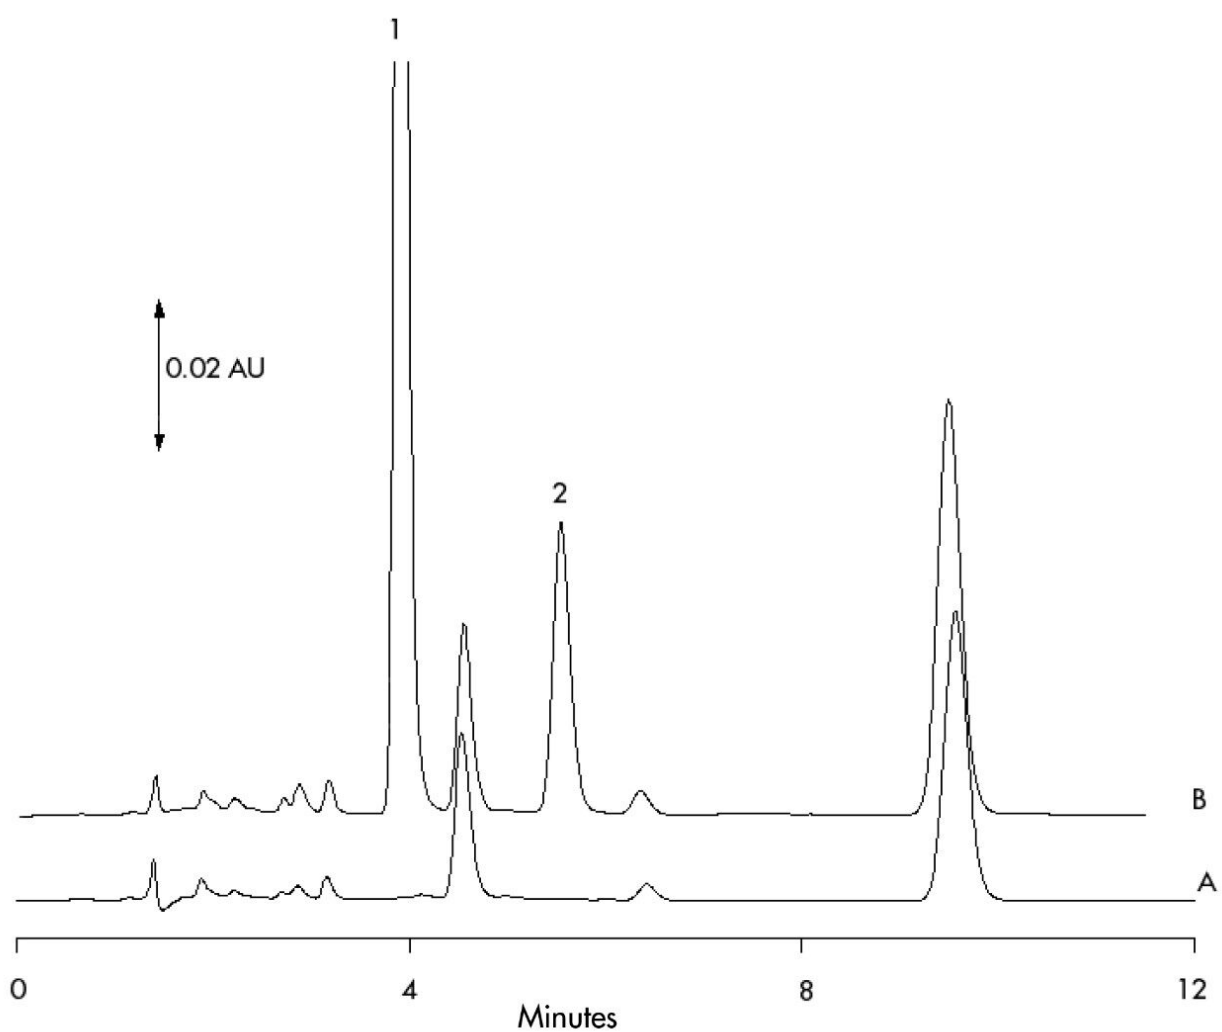

Chromatogram of Serum Extracts: A) Blank B) Spiked Sample.

Featured Products

WA31763.144, June 2003

© 2021 Waters Corporation. All Rights Reserved.