

Nota applicativa

Steroids - 2.1 x 20 mm Intelligent Speed Separation

Waters Corporation



This is an Application Brief and does not contain a detailed Experimental section.


Abstract

This application brief demonstrates analysis of steroids using 2.1 x 20 mm Intelligent Speed Separation Column.


Introduction

The compounds used in this study are –


1. Prednisolone
2. Cortisone
3. Corticosterone
4. Estradiol
5. Estrone
6. Progesterone

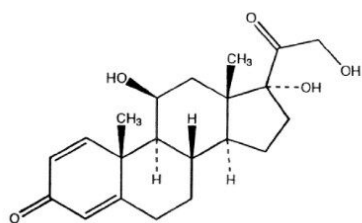


1. Prednisolone

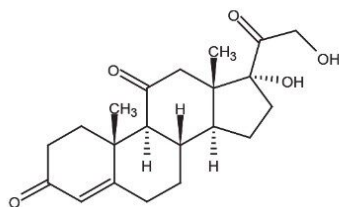


2. Cortisone

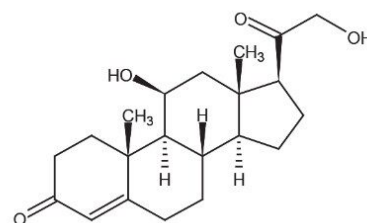


3. Corticosterone



4. Estradiol

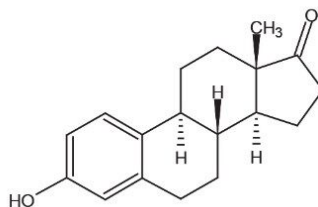

5. Estrone

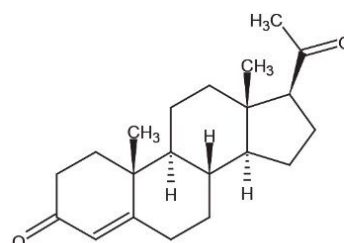

6. Progesterone

Experimental

HPLC Method

Column: Symmetry C₁₈, 2.1 x 20 mm, 3.5 µm IS

Part numbers: 186002066

Mobile phase A: Water

Mobile phase B: ACN

Flow rate: 0.6 mL/min

Injection volume: 5 µL


Temperature: 30 °C

Detection: UV @ 220 nm

Gradient

Time (min)	Profile	
	%A	%B
0	80	20
4	36	64

Results and Discussion

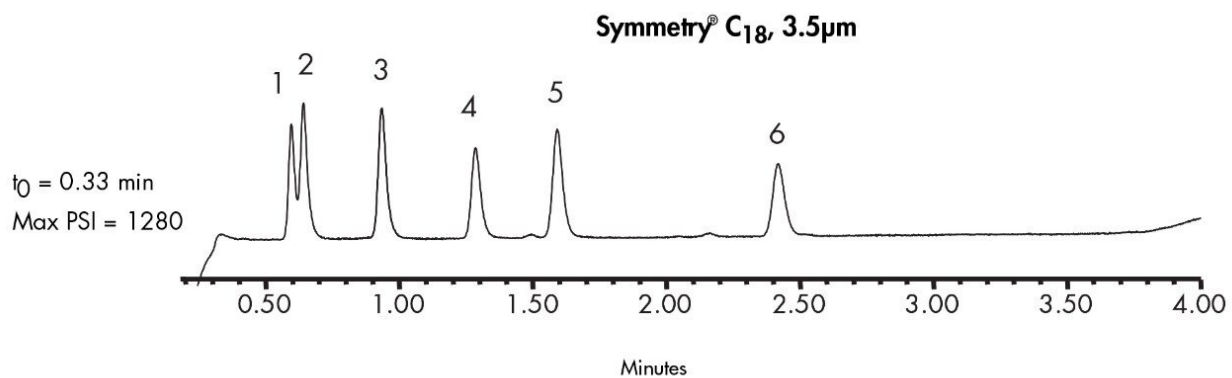

WA31763.151, June 2003