

## Atrazine and Metabolites in Drinking Water

---

Waters Corporation

This is an Application Brief and does not contain a detailed Experimental section.

---

### Abstract

This application brief details on the analysis of atrazine and its metabolites using Symmetry Columns.

---

### Introduction

The compounds analyzed in this study are:

1. Hydroxydesisopropylatrazine
  2. Desethyldeisopropylatrazine
  3. Hydroxydesethylatrazine
  4. Desisopropylatrazine
  5. Hydroxyatrazine
  6. Desethylatrazine
  7. Atrazine
-

---

## Experimental

### HPLC Method

Column:	Symmetry Shield RP <sub>18</sub> , 3.9 x 150 mm, 5 µm
Part number:	186000108
Mobile phase A:	20 mM Phosphate buffer, pH 6.8
Mobile phase B:	Acetonitrile
Flow rate:	0.8 mL/min
Injection volume:	80 µL
Detection:	PDA (215 nm)


### Gradient

Time (min)	Profile	
	%A	%B
0	95	5
2	95	5
20	30	75

# Oasis® MCX SPE Method

Conditions for Oasis® MCX Cartridge, 6 cc, 150 mg

Part Number 186000256

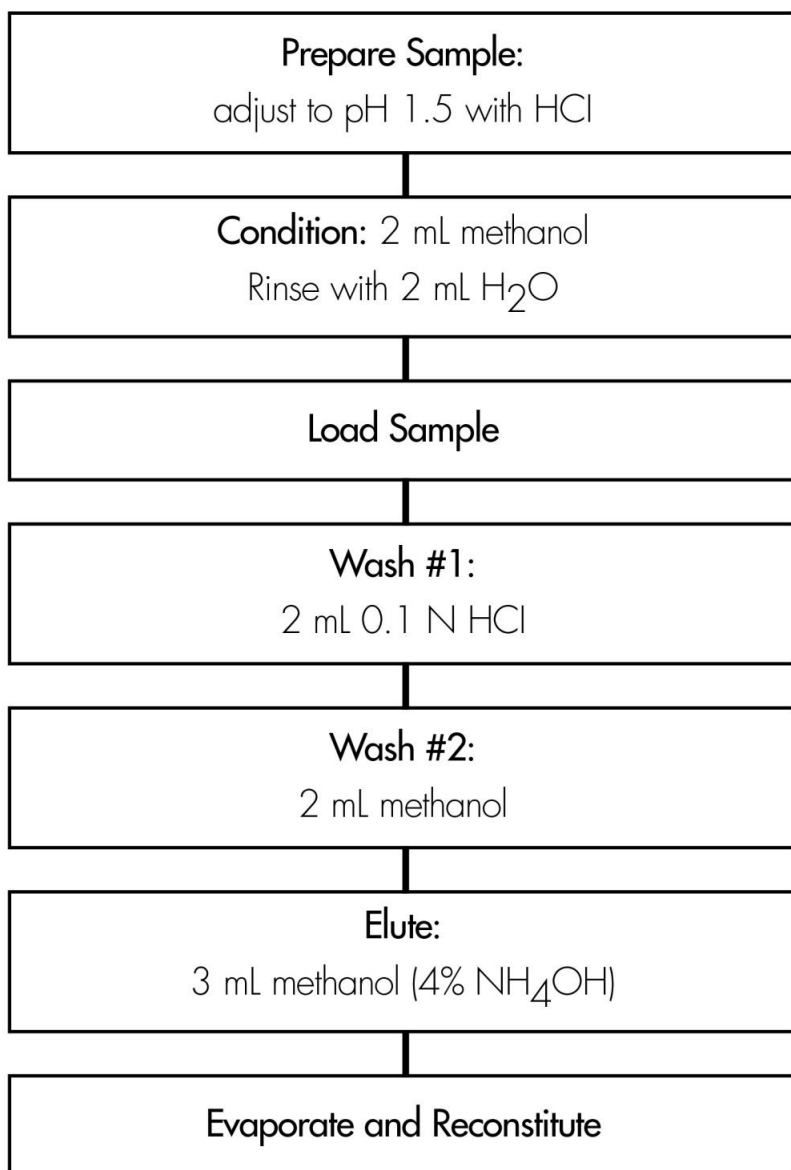


---

## Results and Discussion

Drinking water samples (100 mL) were spiked with the herbicides and adjusted to pH 1.5. The samples were then analyzed using 6 cc Oasis MCX cartridges using the protocol for basic compounds.

Compounds	(% Recovery - % RSD, n=5)	
	0.2 µg/L	1.0 µg/L
1. Hydroxydesisopropylatrazine	94 (3)	85 (3)
2. Desethyl-desisopropylatrazine	75 (8)	76 (5)
3. Hydroxydesethylatrazine	89 (6)	76 (7)
4. Desisopropylatrazine	79 (4)	83 (2)
5. Hydroxyatrazine	107 (7)	101 (2)
6. Desethylatrazine	79 (5)	83 (3)
7. Atrazine	89 (5)	77 (3)

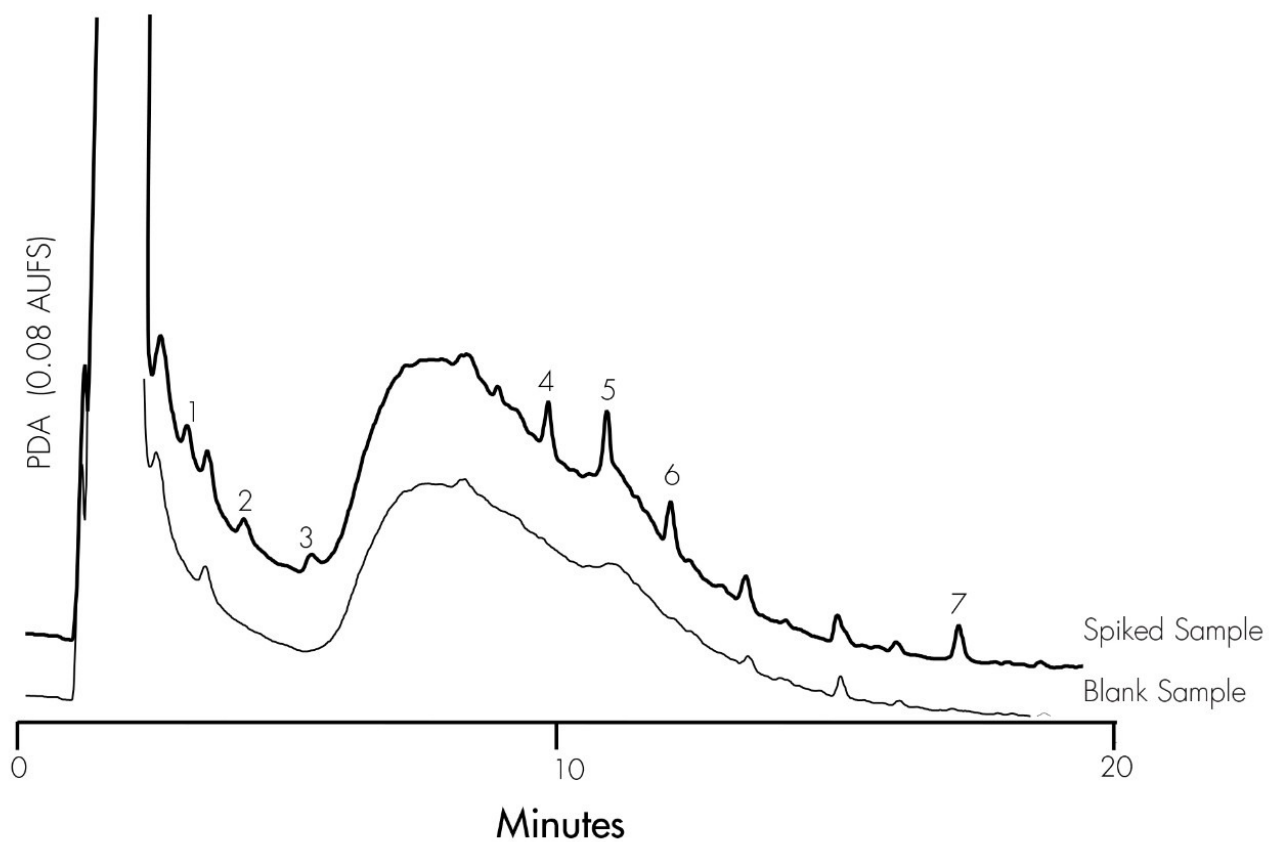

---

## Featured Products

WA31763.32, June 2003

© 2022 Waters Corporation. All Rights Reserved.

---