

Note d'application

Diclofenac

Waters Corporation


This is an Application Brief and does not contain a detailed Experimental section.

Abstract

This application brief demonstrates the analysis of diclofenac using Symmetry Columns.

Introduction

The compound analyzed in this study is diclofenac.

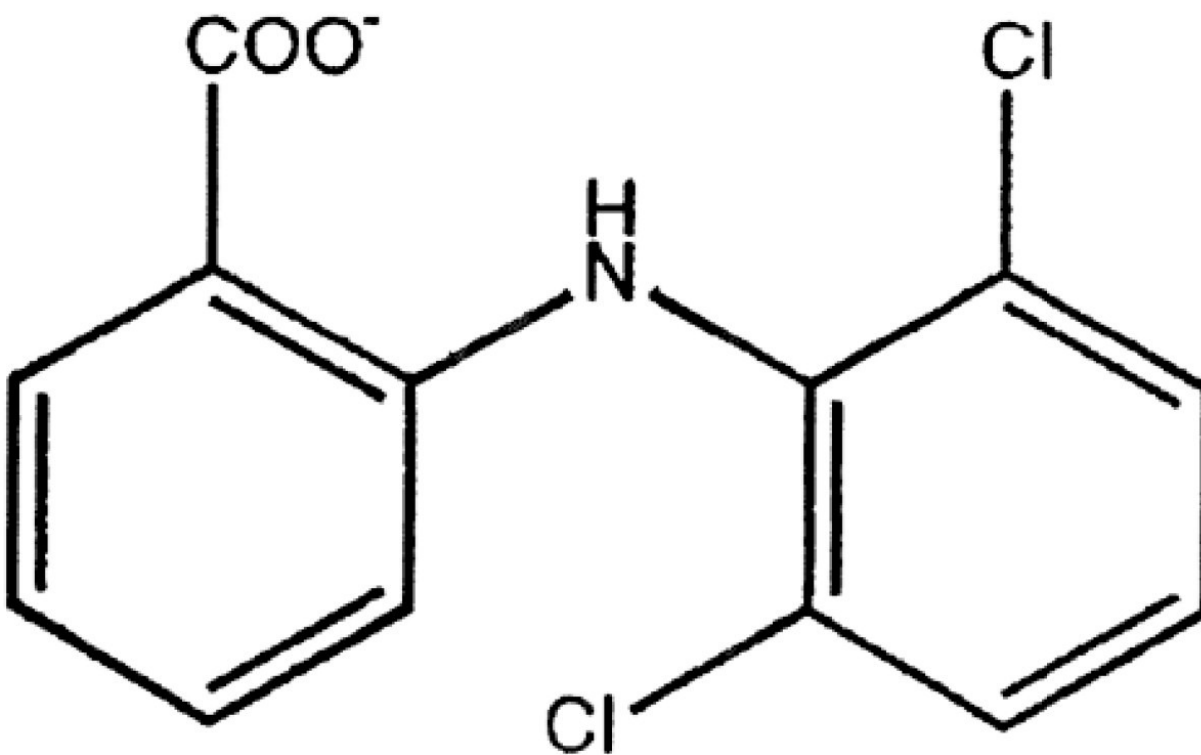

1. Diclofenac

Experimental

HPLC Method

Column:

Symmetry Shield RP₁₈, 4.6 x 150 mm, 5 µm

Part number:


186000109

Mobile phase:	20 mM phosphate buffer, pH 7.0/acetonitrile 65:35
Flow rate:	1.0 mL/min
Injection volume:	5 µL
Detection:	UV @ 220 nm

USP Tailing Factor

1. 1.18

Results and Discussion

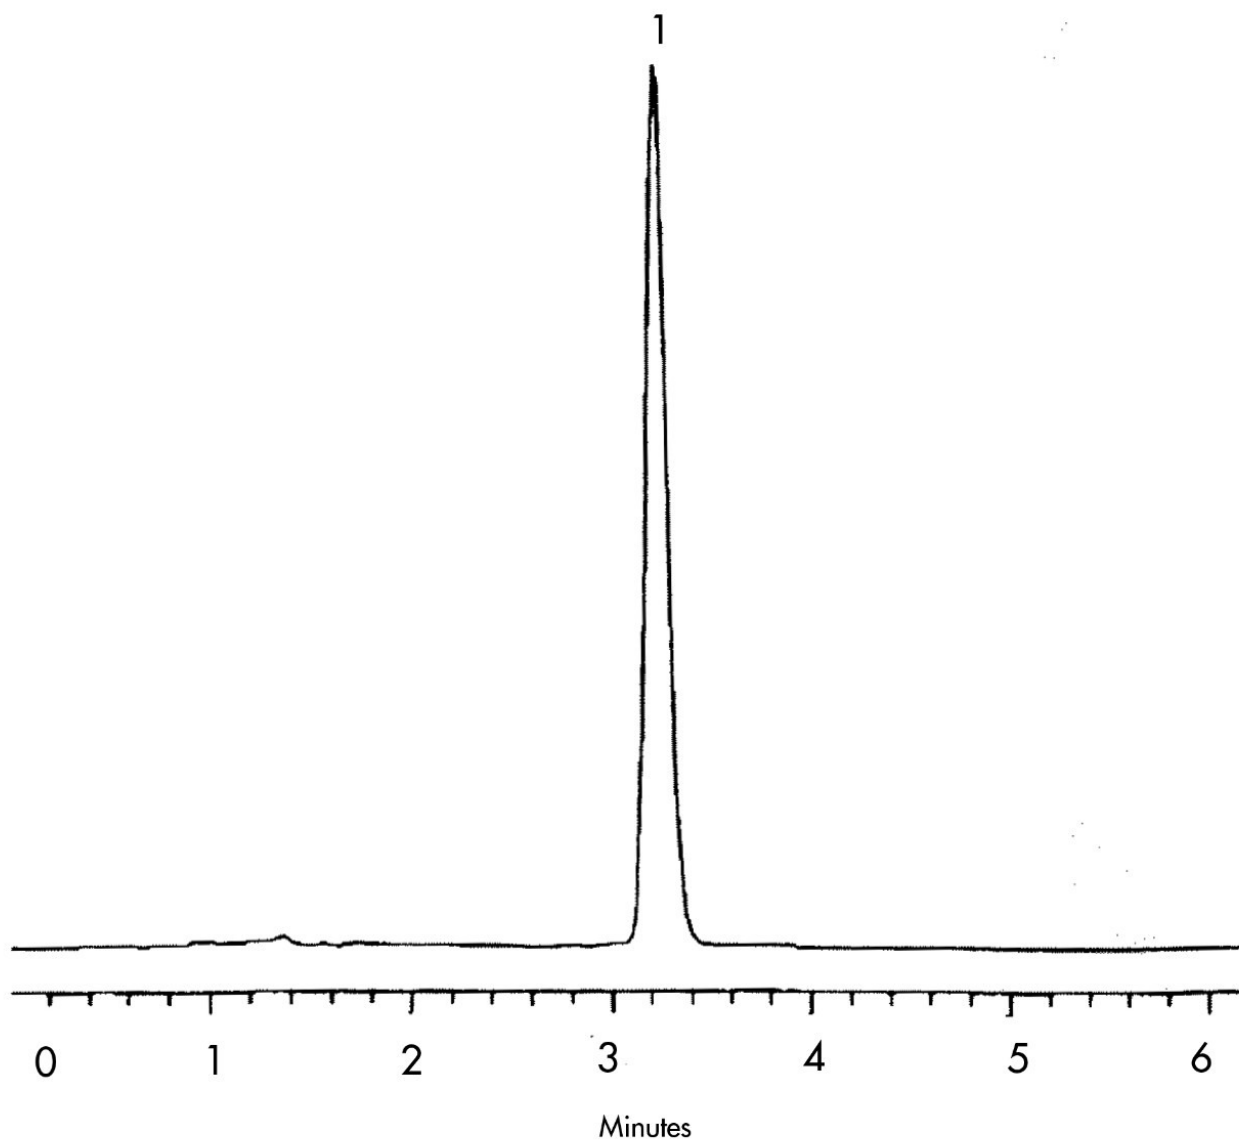

Featured Products

WA31763.73, June 2003

© 2022 Waters Corporation. All Rights Reserved.