

## Trimethoprim in Rat Plasma

---

Waters Corporation




This is an Application Brief and does not contain a detailed Experimental section.

### Abstract

This application brief demonstrates the analysis of Trimethoprim in Rat Plasma using Symmetry Columns.

## Introduction

The compound analyzed in this study is Trimethoprim.

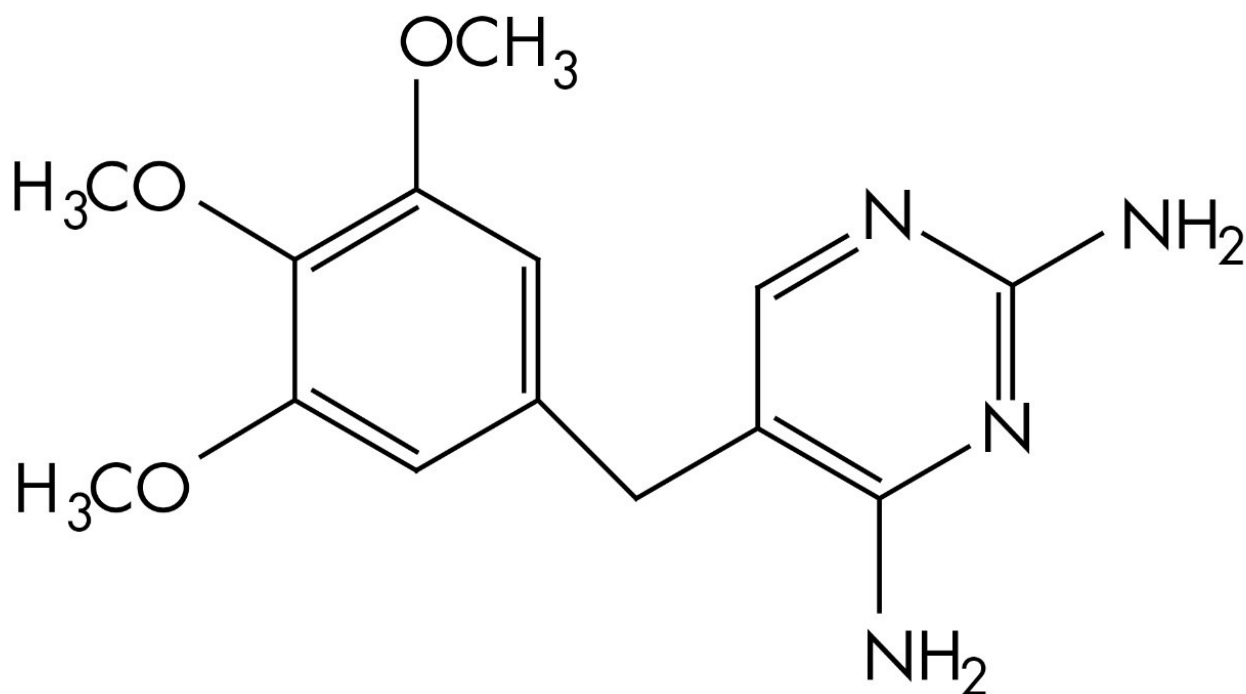

# TRIMETHOPRIM

## Experimental

### HPLC Method

Column:

XTerra MS C<sub>18</sub> 2.1 x 30 mm, 3.5 μm

Part number:

186000398


---

Mobile phase A:	1.0% NH <sub>4</sub> OH
Mobile phase B:	ACN
Isocratic mobile phase composition:	40% A; 60% B
Flow rate:	0.2 mL/min
Injection volume:	30 µL
Detection:	MS ESI+
Instrument:	Alliance 2790, Micromass Quattro Ultima
Ion source:	ESI+
Source temperature:	150 °C
Gas cell:	1.5e <sup>-3</sup> mbar, 25 eV
Desolvation temperature:	350 °C
Cone gas flow:	150 L/hr
Drying gas flow:	600 L/hr
Cone voltage:	20V

# OASIS® MCX EXTRACTION METHOD


Oasis® MCX Extraction Plate, 10 mg/96-well

Part Number 186000259

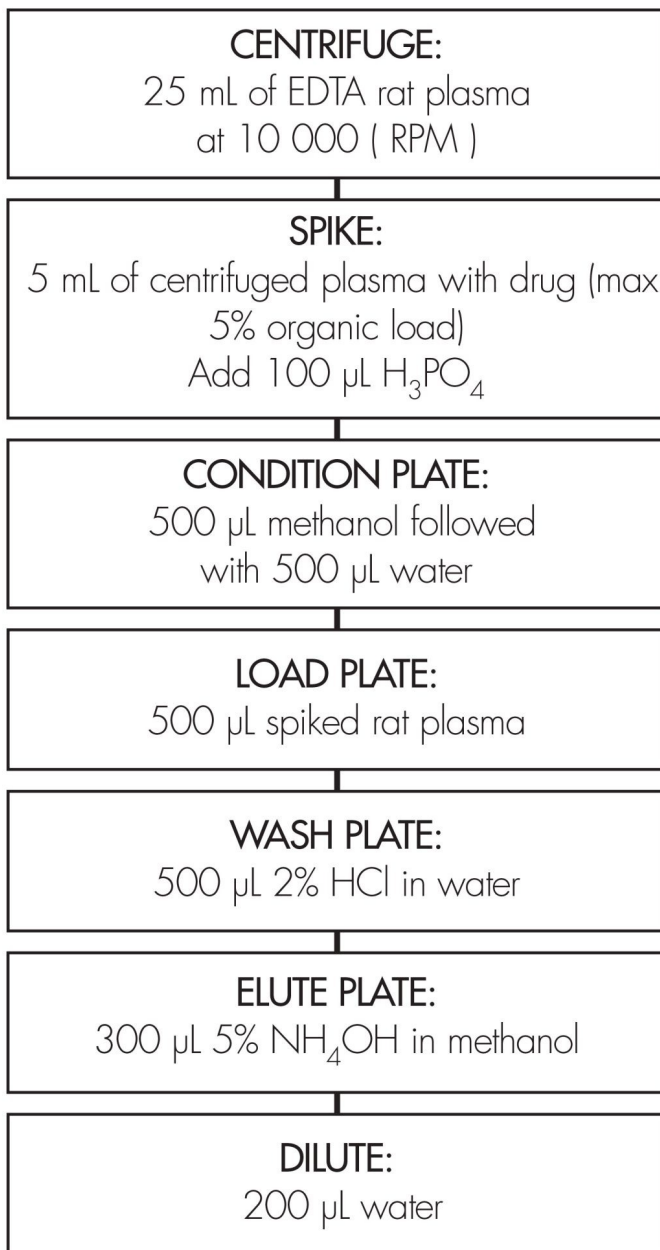


## Results and Discussion

Spike 1 ng/mL, 60/40 ACN/H<sub>2</sub>O 1.0 % NH<sub>4</sub>OH

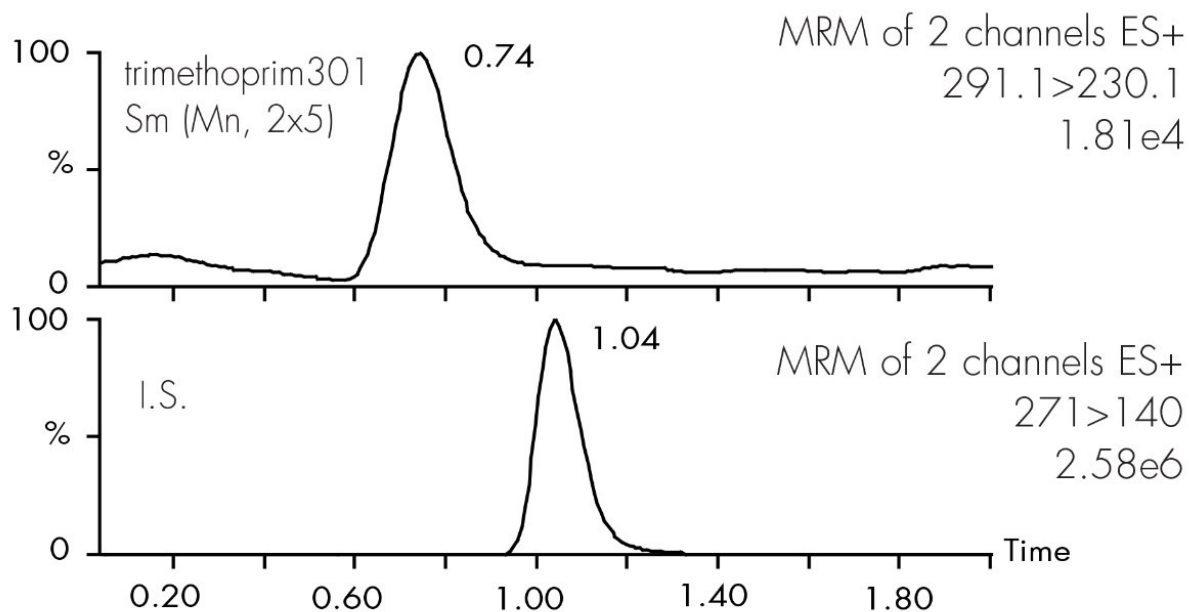

Spike 250 ng/mL, 60/40 ACN/H<sub>2</sub>O 1.0 % NH<sub>4</sub>OH

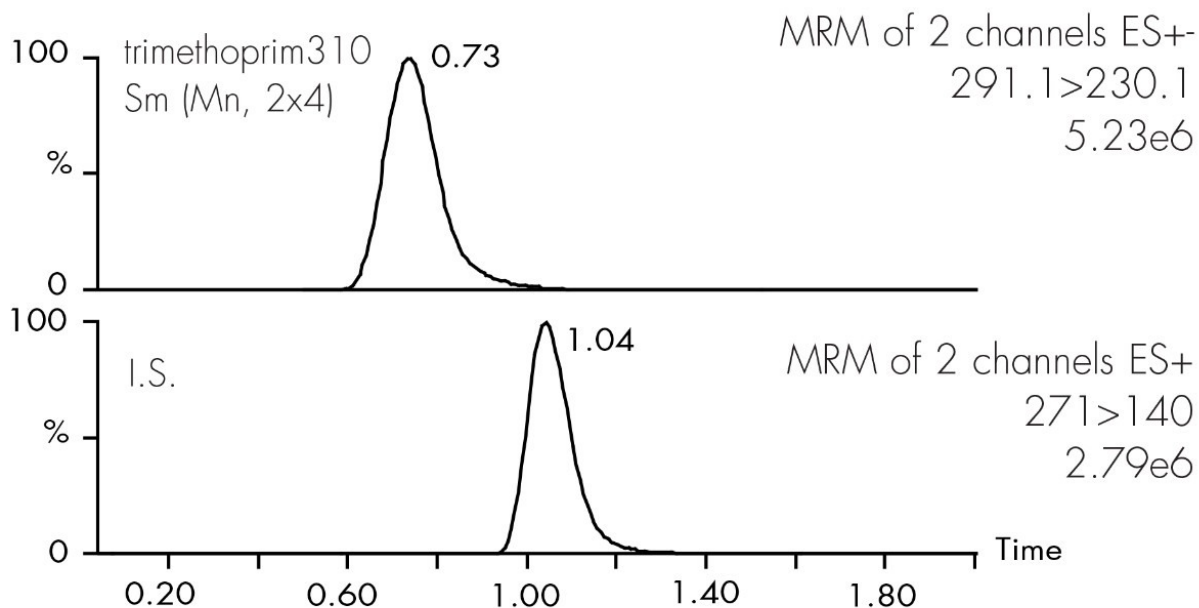

TRIMETHOPRIM (ng/mL)	Mean	Standard deviation	Coefficient of variation (%)	Recovery (%)
1	1.013	0.039	3.9	101
2.5	2.54	0.061	2.4	101
5	4.86	0.18	3.8	97
10	10.015	0.18	1.8	100
20	20.31	0.3	1.5	101
25	24.64	0.76	3.1	98
50	51.62	1.1	2.1	103
100	96.95	0.98	1	96
200	204.13	5.22	2.6	102
250	247.42	4.93	2	98


Compound name: Trimethoprim

Coefficient of Determination: 0.999608

Calibration curve:  $3.83074 \times 10^{-6} \cdot x^2 + 0.00818910 \cdot x + 0.000423977$

Response type: Internal Std (Ref 1), Area\* (IS Conc./IS Area)

Curve type: 2nd Order, Origin: Exclude, Weighting:  $1/x^2$ , Axis trans: None

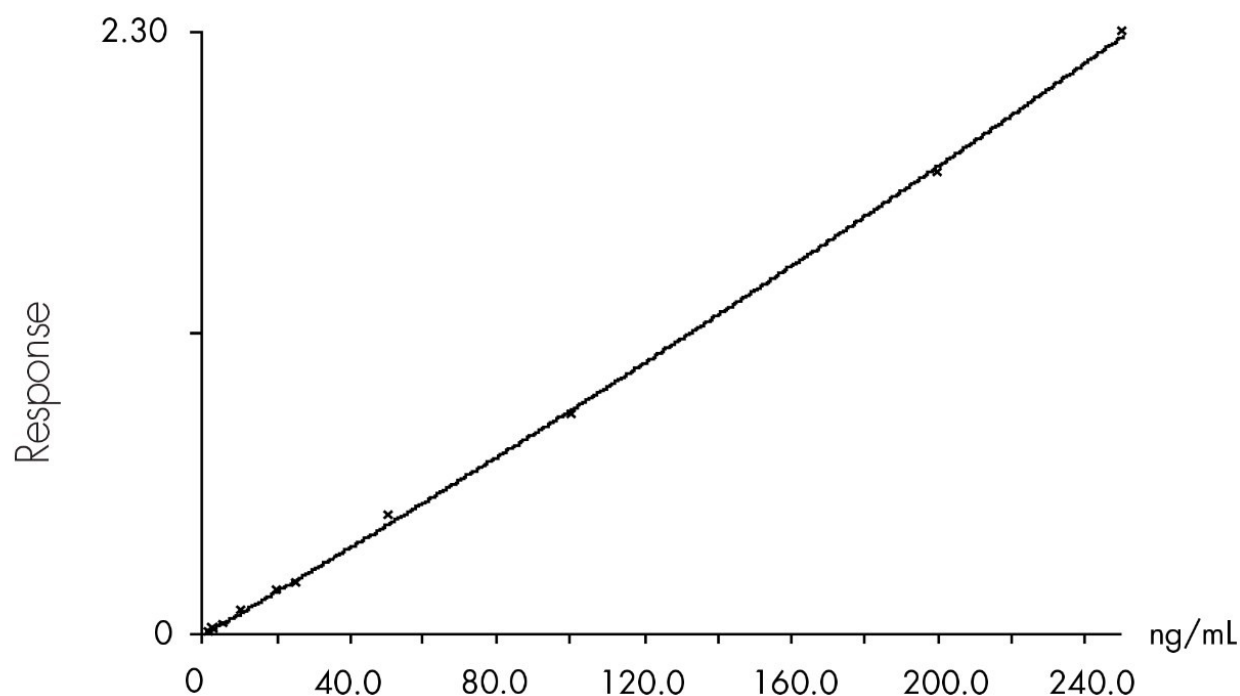

## Featured Products

WA31764.154, June 2003



© 2021 Waters Corporation. All Rights Reserved.