Waters™



Diclofenac in Rat Plasma by LC-MS/MS

Waters Corporation

This is an Application Brief and does not contain a detailed Experimental section.

Abstract

This application brief highlights the analysis of diclofenac in plasma.

Introduction

DICLOFENAC

Experimental

HPLC Method

| Column: | XTerra MS C ₁₈ 2.1 x 30 mm, 3.5 μm | | |
|-------------------------------------|---|--|--|
| Part number: | 186000398 | | |
| Mobile phase A: | 0.05% HCOOH | | |
| Mobile phase B: | ACN | | |
| Isocratic mobile phase composition: | 60% A; 40% B | | |
| Flow rate: | 0.2 mL/min | | |
| Injection volume: | 50 μL | | |
| Detection: | MS ESI | | |
| Instrument: | Alliance 2790, Micromass Quattro Ultima | | |
| lon source: | ESI | | |
| Source temperature: | 150 °C | | |
| Gas cell: | 1.5e ⁻³ mbar, 12 eV | | |
| Desolvation temperature: | 350 °C | | |
| Cone gas flow: | 150 L/hr | | |

Drying gas flow: 600 L/hr

Cone voltage: 30 V

OASIS® MAX EXTRACTION METHOD

Oasis® MAX Extraction Plate, 10 mg/96-well Part Number 186000375

CENTRIFUGE:

25 mL of EDTA rat plasma at 10 000 (RPM)

SPIKE:

5 mL of centrifuged plasma with drug (max 5% organic load) Add 100 μ L H_3PO_4

CONDITION PLATE:

500 µL methanol followed with 500 µL water

LOAD PLATE:

500 µL spiked rat plasma

WASH PLATE:

 $500~\mu L~2~\%~NH_{\rm d}OH~in~water$

ELUTE PLATE:


300 µL 5% HCOOH in methanol

DILUTE:


200 µL water

Results and Discussion

Spike 10 ng/mL, 40/60 ACN/ H_2 O 0.05 % Formic Acid

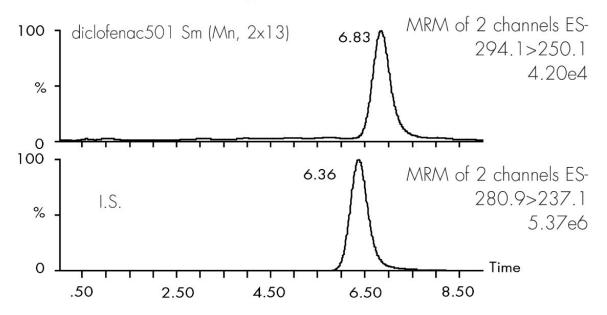

Spike 2001 ng/mL, 40/60 ACN/ H_2O 0.05 % Formic Acid

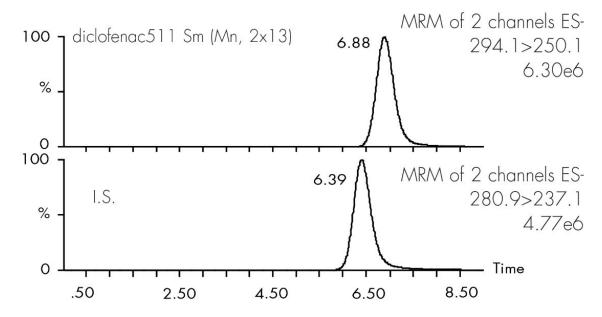

| DICLOFENAC (ng/mL) | mean | Standard deviation | Coefficient of variation (%) | Recovery (%) |
|-----------------------|---------|-----------------------|------------------------------|-----------------|
| 10 | 10.26 | 0.3 | 3 | 102 |
| 25 | 24.06 | 0.83 | 3.5 | 96 |
| 100 | 101.68 | 2.69 | 2.7 | 101 |
| 250 | 250.05 | 8.13 | 3.3 | 100 |
| 500 | 496.41 | 27.09 | 5.5 | 99 |
| 1000 | 997.8 | 28.1 | 2.8 | 99 |
| 1500 | 1497.25 | 27.98 | 1.9 | 99 |


Compound name: Diclofenac

Coefficient of Determination: 0.997049

Calibration curve: $4.68008e-8*x^2 + 0.000702987*x+0.000144152$

Response type: Internal Std (Ref 1), Area* (IS Conc./IS Area)

Curve type: 2nd Order, Origin: Exclude, Weighting: 1/x2, Axis trans: None

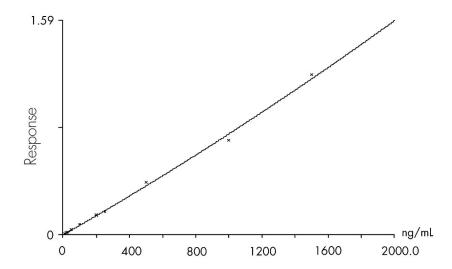

Featured Products

Alliance HPLC System https://www.waters.com/534293

WA31764.70, June 2003

© 2022 Waters Corporation. All Rights Reserved.