


## Separation of a Tryptic Digest of Bovine Hemoglobin

---

Waters Corporation

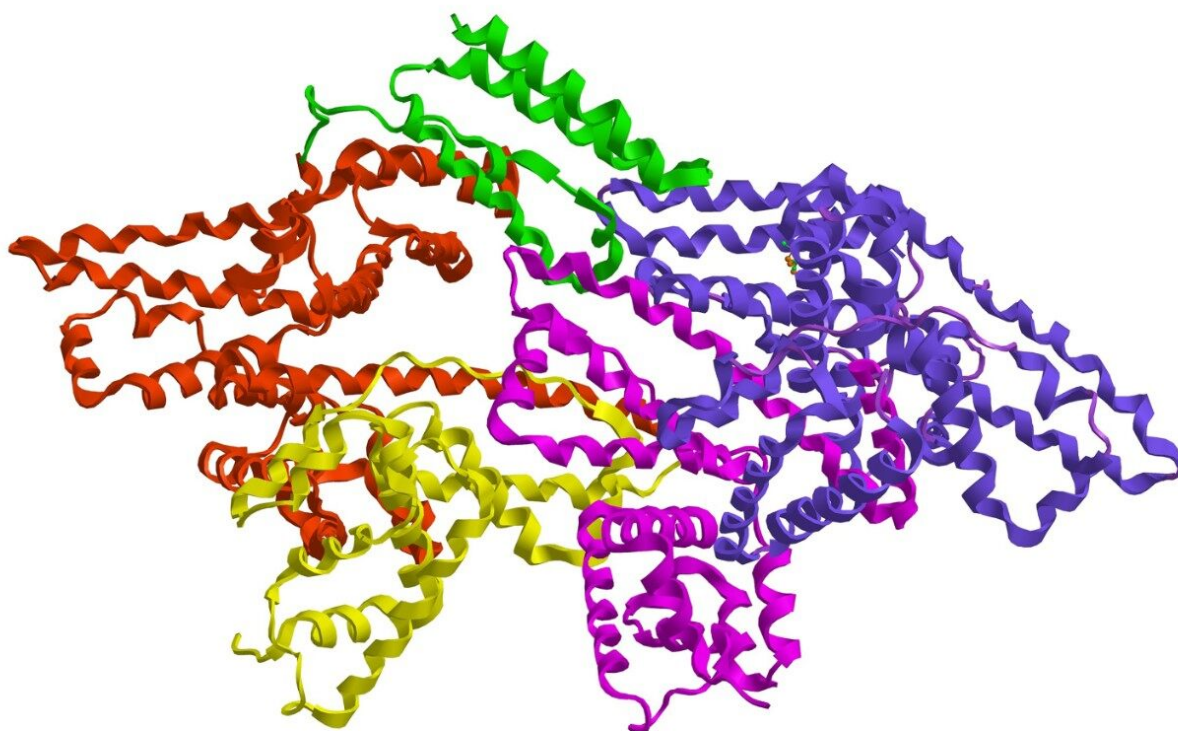

This is an Application Brief and does not contain a detailed Experimental section.

---

### Abstract

This application brief demonstrates separation of a tryptic digest of bovine hemoglobin.

---

## Introduction

The compound used in this study is Bovine haemoglobin.

---


## Experimental

Column:	BioSuite PA-A and PA-B Columns (2.1 x 150 mm)
Eluent A:	0.02% TFA in water
Eluent B:	0.016% TFA in acetonitrile
Gradient:	0–56% B in 70 minutes
Flow rate:	0.16 mL/min
Injection volume:	15 µL
Temperature:	40 °C
Detection:	UV 220 nm

---

## Results and Discussion

Column: BioSuite™ PA-A and PA-B columns (2.1 x 150 mm)  
Eluent A: 0.02% TFA in water  
Eluent B: 0.016% TFA in acetonitrile  
Gradient: 0-56% B in 70 minutes  
Flow rate: 0.16 ml/min  
Injection Volume: 15 µl  
Temperature: 40 °C  
Detection: UV 220 nm

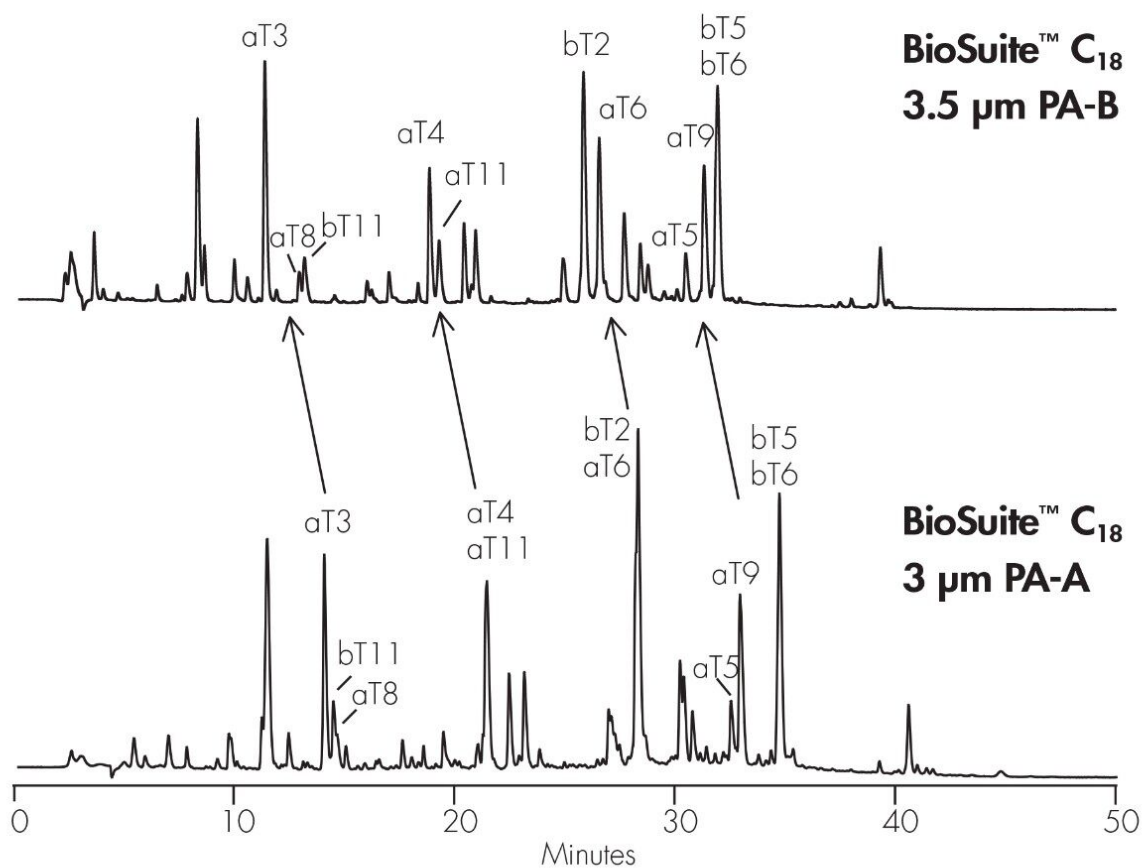

## Featured Products

WA31791, June 2003

