

## Determination of Priority Pesticide Residues in Baby Food by Tandem Quadrupole LC-MS/MS and GC-MS/MS

---

Peter Hancock, Cristiana C. Leandro, Brendan J. Keely, Richard J. Fussell

Waters Corporation, Central Science Laboratory, York



---

## Abstract

The aim was to develop a simple and rapid method suitable for the quantification and confirmation of a total of 25 priority pesticide residues and transformation products in baby foods at a level of 0.001 mg/kg using LC-MS/MS and GC-MS/MS.

---

## Introduction

The European Union Baby Food Directive 2003/13/EC<sup>1</sup> designates pesticides as prohibited, in which case they are considered not to have been used if their residue does not exceed 0.003 mg/kg or have maximum residue limits (MRLs) set between 0.004–0.008 mg/kg. Seven pesticides and nine transformation products (e.g. metabolites) listed in the Directive are suitable for LC-MS analysis while nine pesticides and three transformation products are amenable to GC-MS. The other pesticides specified in the Directive, because of their physicochemical properties, must be analyzed by single residue methods. Dimethoate was only included in the compound list as a possible precursor for omethoate.

To be able to enforce the Directive, laboratories require multiresidue methods with lower limits of detection (LOD) than those currently available. This necessitates improvements in the extraction, clean up, separation, and detection of pesticides in baby food samples. An extraction, with acetonitrile, followed by dispersive SPE clean up was reported for the analysis of a wide range of pesticides in fruits and vegetables<sup>2</sup> and fatty samples.<sup>3</sup> Acetonitrile extracts are suitable for direct analysis using LC-MS/MS, and by GC-MS/MS using programmable temperature vaporization (PTV) in solvent vent mode.

GC and HPLC have both been widely used in laboratories for the analysis of pesticide residues in food. The Waters ACQUITY UltraPerformance LC (UPLC)<sup>4</sup> has the potential to provide shorter run times, greater sensitivity and better chromatographic resolution than established HPLC methods.

---

## Experimental

### Extraction Method

10 g of baby food was weighed in a centrifuge tube. For recovery, the samples were spiked at 0.001 mg/kg. Acetonitrile (10 mL), anhydrous MgSO<sub>4</sub> (4 g) and NaCl (1 g) were added and the tube was shaken and vortexed immediately. For the GC-MS/MS experiments, 100 µL of 1 µg/mL δ-HCH was added as an internal standard. After centrifugation at 4300 g for 5 minutes, an aliquot (1 mL) of the supernatant was transferred to a microcentrifuge vial containing 50 mg primary secondary amine (PSA) sorbent and 150 mg anhydrous MgSO<sub>4</sub>. For the GC-MS/MS experiments, 200 mg C<sub>18</sub> was also added to the microcentrifuge vial. The contents were vortex mixed for 30 s and centrifuged at 5000 g for 1 minute. The supernatant was analyzed by LC-MS/MS after dilution with water (1:10) or directly by GC-MS/MS.

## HPLC Conditions

System:	Waters Alliance 2795 Separations Module
Column:	SunFire C <sub>18</sub> , 2.1 x 100 mm, 3.5 µm
Column temp.:	40 °C
Flow rate:	0.3 mL/min
Mobile phase A:	H <sub>2</sub> O:MeOH (9:1) + 20 mM CH <sub>3</sub> CO <sub>2</sub> NH <sub>4</sub>
Mobile phase B:	H <sub>2</sub> O:MeOH (1:9) + 20 mM CH <sub>3</sub> CO <sub>2</sub> NH <sub>4</sub>
Injection volume	50 µL

## Gradient

Time: 0 min	100% A
Time: 13 min	100% B
Time: 17 min	100% B

## UPLC Conditions

System:	Waters ACQUITY UltraPerformance LC System
Column:	UPLC BEH C <sub>18</sub> , 2.1 x 100 mm, 1.7 μm
Column temp.:	40 °C
Flow rate:	0.3 mL/min
Mobile phase A:	H <sub>2</sub> O:MeOH (9:1) + 20 mM CH <sub>3</sub> CO <sub>2</sub> NH <sub>4</sub>
Mobile phase B:	H <sub>2</sub> O:MeOH (1:9) + 20 mM CH <sub>3</sub> CO <sub>2</sub> NH <sub>5</sub>
Injection volume:	50 μL

## Gradient

Time: 0 min	100% A
Time: 5 min	100% B
Time: 7 min	100% B

## GC Conditions

System:	Agilent 6890 GC with 7683 autosampler
Column:	Varian FactorFour VF-5ms 30 m x 0.25 mm i.d., 0.25 μm
Constant flow:	1.0 mL/min helium
Injection method:	Cyro cooled PTV in solvent vent mode, 5 μL injected

Vent method: Vent pressure 5 kPa, Vent flow 20 mL/min for 0.5 min

### Temp. ramp:

Time: 0 min 50 °C

Time: 1.5 min 50 °C

Time: 9 min 200 °C

Time: 11 min 200 °C

Time: 15 min 280 °C

### LC-MS/MS Method

The Waters Micromass Quattro Premier XE Tandem Quadrupole Mass Spectrometer was used in positive ion electrospray mode. The ion source was operated at 120 °C with a capillary voltage of 3.5 kV. The mode of acquisition was multiple reaction monitoring (MRM) at an argon collision gas pressure of  $3.0 \times 10^{-3}$  mBar.

The Quattro Premier XE was tuned so that the precursor and product ions were resolved with a peak width at half height of less than 0.7 Da. The list of pesticide residues and the MRM transitions, along with the cone voltages and collision energies for the method are listed in Table 1.

Pesticide (Collision Energy)	Quantification Transition (Collision Energy)	Confirmation Transition	Cone Voltage
Omethoate	214 > 183 (12 eV)	214 > 155 (16 eV)	20 V
Oxydemeton-s-methyl	247 > 169 (14 eV)	247 > 109 (28 eV)	20 V
Demeton-s-methylsulfone	263 > 169 (17 eV)	263 > 121 (17 eV)	26 V
Dimethoate	230 > 125 (20 eV)	230 > 171 (15 eV)	13 V
Fensulfothion-oxon	293 > 237 (19 eV)	293 > 265 (14 eV)	28 V
Fensulfothion-oxon-sulfone	309 > 253 (16 eV)	309 > 175 (27 eV)	27 V
Demeton-s-methyl	231 > 89 (12 eV)	231 > 61 (30eV)	12 V
Disulfoton sulfoxide	291 > 185 (14 eV)	291 > 97 (31 eV)	18 V
Disulfoton sulfone	307 > 97 (29 eV)	307 > 115 (24 eV)	23 V
Fensulfothion	309 > 281 (15 eV)	309 > 157 (25 eV)	29 V
Fensulfothion sulfone	325 > 269 (16 eV)	325 > 297 (11 eV)	26 V
Terbufos sulfone	321 > 171 (12 eV)	321 > 115 (29 eV)	21 V
Terbufos sulfoxide	305 > 187 (11 eV)	305 > 131 (28 eV)	14 V
Ethoprophos	243 > 131 (20 eV)	243 > 173 (15eV)	20 V
Disulfoton	275 > 89 (10 eV)	275 > 61 (33 eV)	9 V
Cadusafos	271 > 159 (15 eV)	271 > 131 (23 eV)	18 V
Terbufos	289 > 103 (9 eV)	289 > 233 (5 eV)	12 V

Table 1. LC-MS/MS MRM method parameters.

## GC-MS/MS Method

The Waters Micromass Quattro micro<sup>TM</sup> GC Tandem Quadrupole Mass Spectrometer was used in electron impact (EI+) mode. The ion source was operated at 180 °C with an electron energy of 70 eV and a trap current of 200 µA. The mode of acquisition was multiple reaction monitoring (MRM) at an argon collision gas pressure of  $3.0 \times 10^{-3}$  mBar.

The Quattro micro GC was tuned so that the precursor and product ions were resolved with a peak width at half height of less than 0.7 Da. The list of pesticide residues and the MRM transitions, along with the collision energies for the method are listed in Table 2.

<b>Pesticide (Collision Energy)</b>	<b>Quantification Transition (Collision Energy)</b>	<b>Confirmation Transition</b>
Omethoate	156 > 110 (10 eV)	156 > 79 (20 eV)
Ethoprophos	158 > 114 (5 eV)	200 > 158 (5 eV)
Cadusafos	159 > 131 (8 eV)	158 > 114 (5 eV)
Hexachlorobenzene	284 > 249 (15 eV)	286 > 251 (15 eV)
Dimethoate	125 > 79 (8 eV)	229 > 87 (5 eV)
Fipronil de-sulfinyl	388 > 333 (20 eV)	333 > 281 (10 eV)
$\delta$ -HCH, Internal Standard	219 > 183 (5 eV)	183 > 145 (15eV)
Heptachlor	272 > 237 (13 eV)	274 > 239 (15 eV)
Aldrin	263 > 193 (25 eV)	263 > 191 (25 eV)
Fipronil	367 > 213 (22 eV)	369 > 215 (25 eV)
Heptachlor epoxide	183 > 155 (10 eV)	217 > 182 (15 eV)
Dieldrin	263 > 193 (25 eV)	263 > 191 (25 eV)
Nitrofen	283 > 253 (10 eV)	283 > 162 (20 eV)
Endrin	263 > 193 (25 eV)	263 > 191 (25 eV)

Table 2. GC-MS/MS MRM method parameters.

## Acquisition and Processing Methods

The data were acquired using Waters MassLynx Software and processed using the Waters TargetLynx Application Manager. Two MRM transitions were acquired for each residue so that quantification and confirmation could be performed with a single injection assuming that the ion ratio between the two transitions was consistent for standards and samples. The confirmation criteria chosen were dependent on the relative abundance of the two transitions in accordance with EU legislation 2002/657/EC<sup>5</sup> usually applied to veterinary drug residues analysis.

## Results and Discussion

### HPLC-MS/MS

To test the extraction method described, seven recovery experiments were performed in fruit-based, potato-based, and cereal-based baby foods, spiked at 0.001 mg/kg. The mean recovery and relative standard

deviation (% RSD) in parenthesis of each analyte are listed in Table 3.

<b>Pesticide Residue</b>	<b>Fruit</b>	<b>Potato</b>	<b>Cereal</b>
Cadusafos	105 (4)	100 (4)	105 (2)
Demeton-s-methyl	113 (5)	104 (4)	98 (5)
Demeton-s-methylsulfone	104 (4)	105 (6)	103 (3)
Dimethoate	107 (2)	106 (7)	104 (4)
Disulfoton	89 (17)	100 (13)	106 (13)
Disulfoton sulfone	106 (6)	103 (1)	102 (3)
Disulfoton sulfoxide	105 (4)	106 (4)	103 (3)
Ethoprophos	107 (2)	103 (3)	103 (4)
Fensulfothion	107 (5)	98 (5)	106 (3)
Fensulfothion-oxon	106 (2)	102 (5)	103 (4)
Fensulfothion-oxon-sulfone	109 (4)	102 (4)	105 (4)
Fensulfothion sulfone	105 (4)	102 (5)	104 (2)
Omethoate	98 (2)	90 (2)	97 (3)
Oxydemeton-s-methyl	105 (6)	101 (4)	110 (3)
Terbufos	108 (14)	85 (10)	98 (6)
Terbufos sulfone	108 (4)	103 (5)	107 (5)
Terbufos sulfoxide	110 (3)	99 (4)	106 (4)

Excellent recoveries in the range 85–113% with % RSDs of less than 17% were obtained by HPLC-MS/MS for all the pesticides spiked at the 0.001 mg/kg levels in three different baby foods.

Calibration curves were linear over the range 0.0005–0.0100 µg/mL with correlation coefficients greater than



0.99 for all analytes using HPLC-MS/MS.

With HPLC-MS/MS all pesticides except disulfoton and terbufos could be confirmed at the 0.001 mg/kg level with a signal-to-noise (S/N) ratio of at least 3:1. The confirmation of the identity of pesticides was based on the ion ratio statistics for the transitions monitored<sup>5</sup>. Table 4 shows the ion ratio statistics for 21 recovery experiments across the three matrices.

<b>Pesticide Residue and Cereal</b>	<b>Fruit, Potato Tolerance</b>	<b>2002/657/EC<sup>5</sup></b>
Cadusafos	0.590 (5)	20
Demeton-s-methyl	0.073 (14)	30
Demeton-s-methylsulfone	0.377 (7)	25
Dimethoate	0.780 (6)	20
Disulfoton	0.078 (36)	50
Disulfoton sulfone	0.096 (10)	50
Disulfoton sulfoxide	0.622 (4)	20
Ethoprophos	0.869 (4)	20
Fensulfothion	0.978 (6)	20
Fensulfothion-oxon	0.732 (5)	20
Fensulfothion-oxon-sulfone	0.423 (7)	20
Fensulfothion sulfone	0.418 (5)	25
Omethoate	0.862 (3)	20
Oxydemeton-s-methyl	0.507 (6)	20
Terbufos	0.248 (32)	25
Terbufos sulfone	0.443 (7)	25
Terbufos sulfoxide	0.257 (6)	25

Table 4. Ion ratios using HPLC-MS/MS for 0.001 mg/kg recovery samples in three different matrices (n = 21).

With the exception of disulfoton and terbufos, the % RSDs indicate good repeatability within the tolerances specified in the EU legislation. For these two compounds, the response for the second transition is not adequate for the confirmation at the MRL level.

Since they are both late eluting compounds, the confirmation could be achieved by injecting crude extracts (e.g. 20  $\mu$ L of the total extract prior to dilution) to load more analyte into the column, without compromising the peak shape.

## UPLC-MS/MS

To test the extraction method described, seven recovery experiments were performed in fruit-based, potato-based and cereal-based baby foods, spiked at mg/kg. The mean recovery and relative standard deviation (% RSD) in parenthesis of each analyte are listed in Table 5.

<b>Pesticide Residue</b>	<b>Fruit</b>	<b>Potato</b>	<b>Cereal</b>
Cadusafos	101 (2)	98 (6)	102 (3)
Demeton-s-methyl	101 (4)	101 (3)	105 (2)
Demeton-s-methylsulfone	119 (3)	116 (4)	119 (2)
Dimethoate	96 (6)	100 (3)	102 (7)
Disulfoton	98 (7)	97 (11)	93 (10)
Disulfoton sulfone	105 (5)	104 (4)	100 (5)
Disulfoton sulfoxide	102 (4)	99 (6)	104 (6)
Ethoprophos	98 (4)	99 (2)	103 (5)
Fensulfothion	103 (5)	104 (5)	101 (5)
Fensulfothion-oxon	101 (4)	100 (3)	104 (6)
Fensulfothion-oxon-sulfone	106 (4)	96 (8)	106 (4)
Fensulfothion sulfone	102 (5)	104 (5)	112 (5)
Omethoate	92 (4)	94 (9)	95 (5)
Oxydemeton-s-methyl	96 (8)	96 (4)	97 (6)
Terbufos	94 (10)	97 (9)	93 (6)
Terbufos sulfone	103 (4)	102 (6)	103 (5)
Terbufos sulfoxide	106 (4)	101 (2)	101 (5)

*Table 5. Mean recovery and % RSD using UPLC-MS/MS for 0.001 mg/kg recovery samples (n = 7).*

Excellent recoveries in the range 92–119% with %RSDs of less than 11% were obtained by UPLC-MS/MS for all the pesticides spiked at the 0.001 mg/kg levels in three different baby foods. Although the mean recoveries obtained by HPLC and UPLC are very similar, the precision obtained with UPLC is significantly

improved, especially for disulfoton and terbufos.

Calibration curves were linear over the range 0.0005–0.0100 µg/mL with correlation coefficients greater than 0.99 for all analytes using UPLC-MS/MS.

With UPLC-MS/MS all pesticides could be confirmed at the 0.001 mg/kg level with a signal-to-noise (S/N) ratio of at least 3:1. Table 6 shows the ion ratio statistics for 21 recovery experiments across the three matrices.

<b>Pesticide Residue</b>	<b>Fruit and Potato (% RSD)</b>	<b>2002/657/EC5</b>
Aldrin	0.645 (10)	20
Cadusafos	0.364 (10)	25
Dieldrin	0.621 (10)	20
Dimethoate	0.240 (20)	25
Endrin	0.650 (9)	20
Ethoprophos	0.992 (7)	20
Fipronil	0.784 (8)	20
Fipronil de-sulfinyl	0.834 (9)	20
Heptachlor	0.593 (9)	20
Heptachlor epoxide	0.781 (14)	20
Hexachlorobenzene	0.674 (6)	20
Nitrofen	0.846 (11)	20
Omethoate	0.518 (10)	20

Table 6. Ion ratios using UPLC-MS/MS for 0.001 mg/kg recovery samples in three different matrices (n = 21).

The % RSDs indicate good repeatability within the tolerances specified in the EU legislation. Notably, the analysis by UPLC-MS/MS overcame the problem of confirming disulfoton and terbufos owing to the improved response.

The peak width of peaks from UPLC is less than those from HPLC, which typically results in increased S/N. See Figure 1. Consequently, UPLC allows confirmation of all the pesticides according to the maximum permitted tolerances for ion ratios.

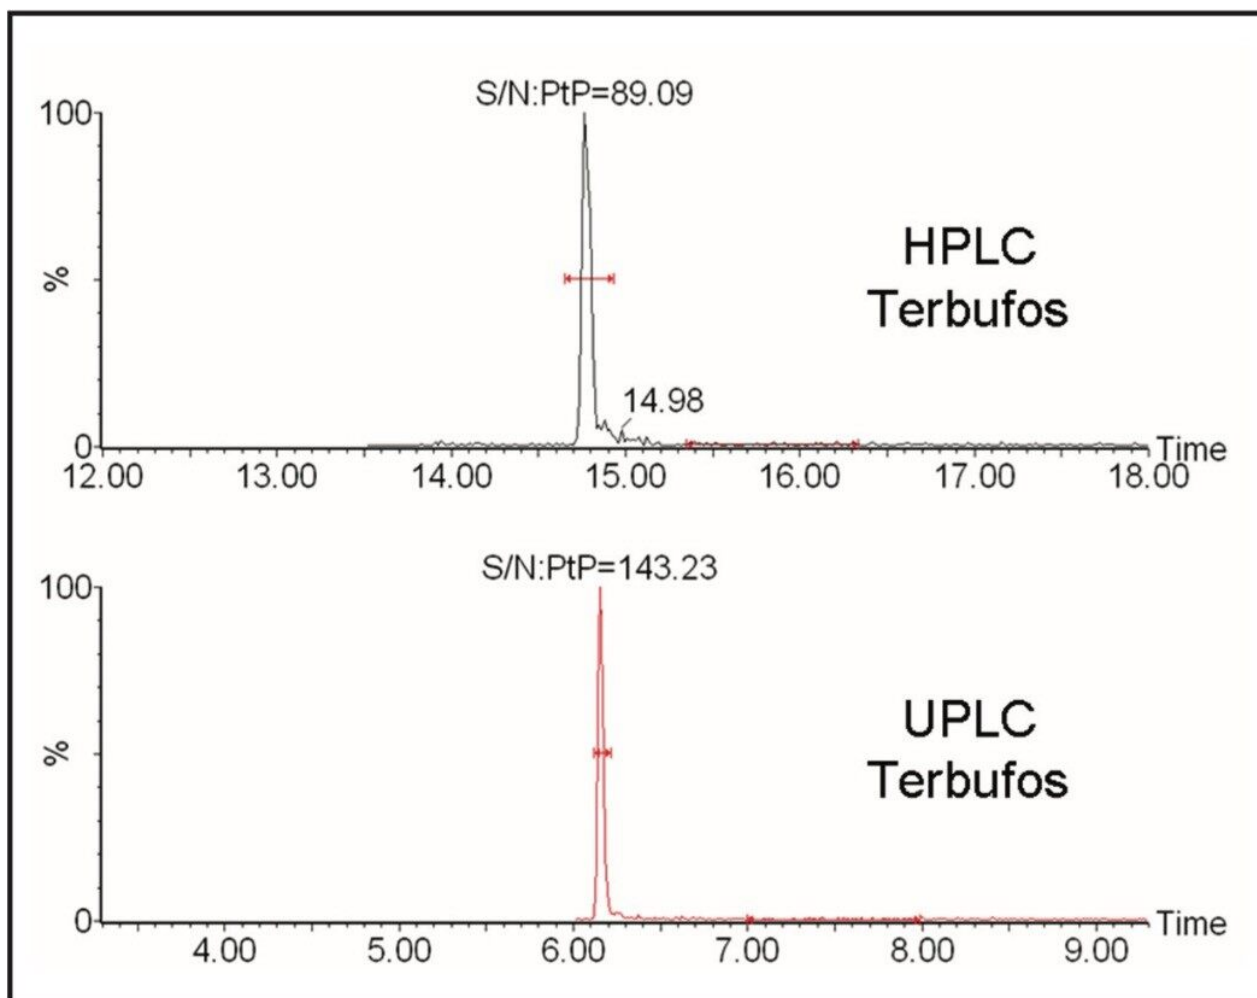


Figure 1. Comparison of S/N obtained for terbufos from HPLC and UPLC.

Converting the method from HPLC to UPLC has other potential advantages, namely improved speed and resolution. The UPLC analysis is complete in less than 10 minutes against the 25 minutes analysis by HPLC. See Figure 2.

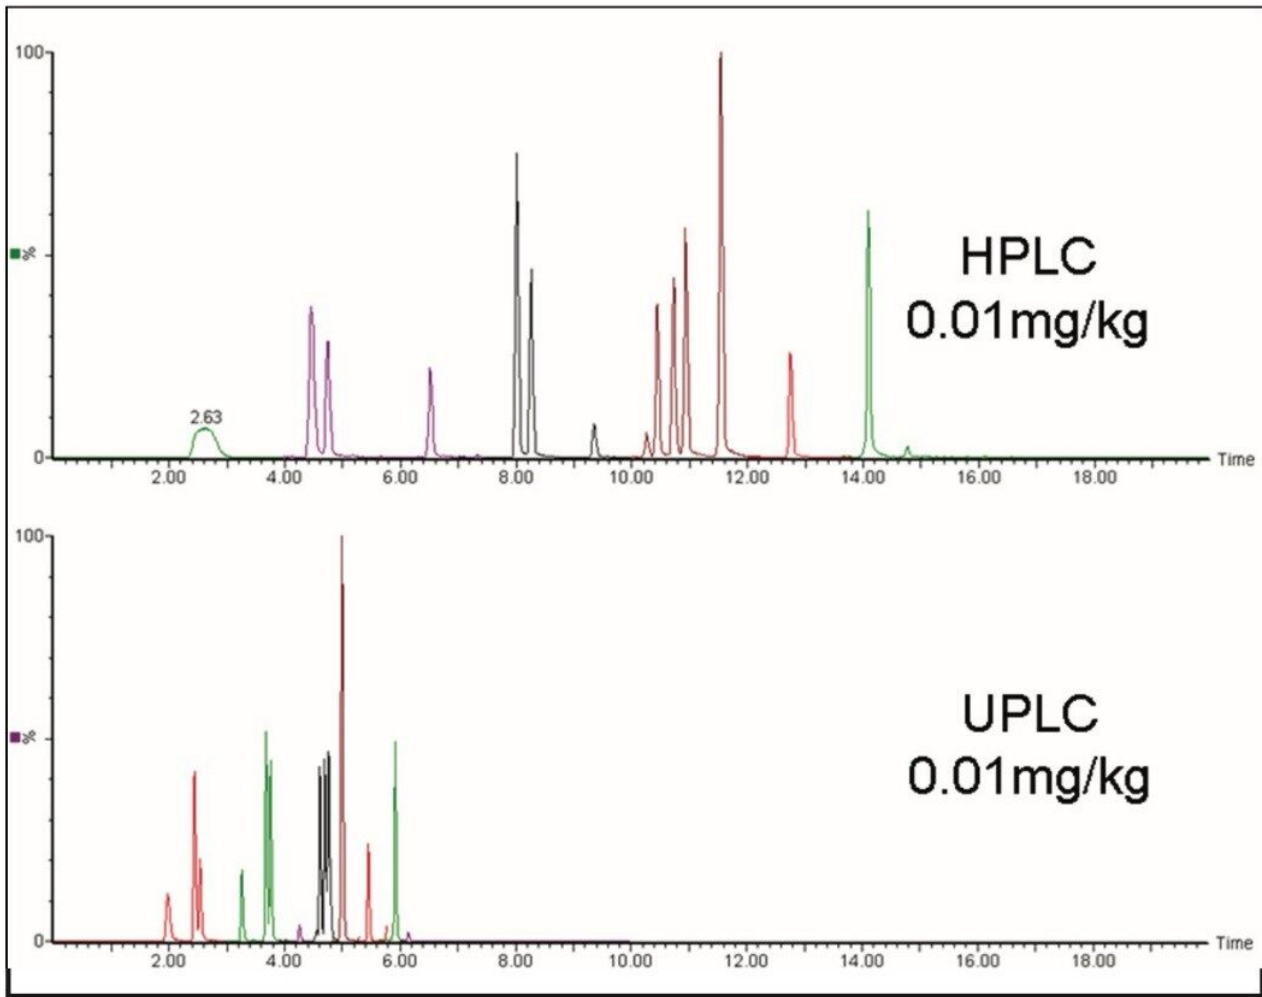


Figure 2. Comparison of run times between HPLC and UPLC for a cereal-based baby food.

The high efficiency of the separation using a 1.7  $\mu\text{m}$  particle size results in a reduction of the peak width, e.g. for terbufos sulfone the peak width is reduced. See Figure 3.

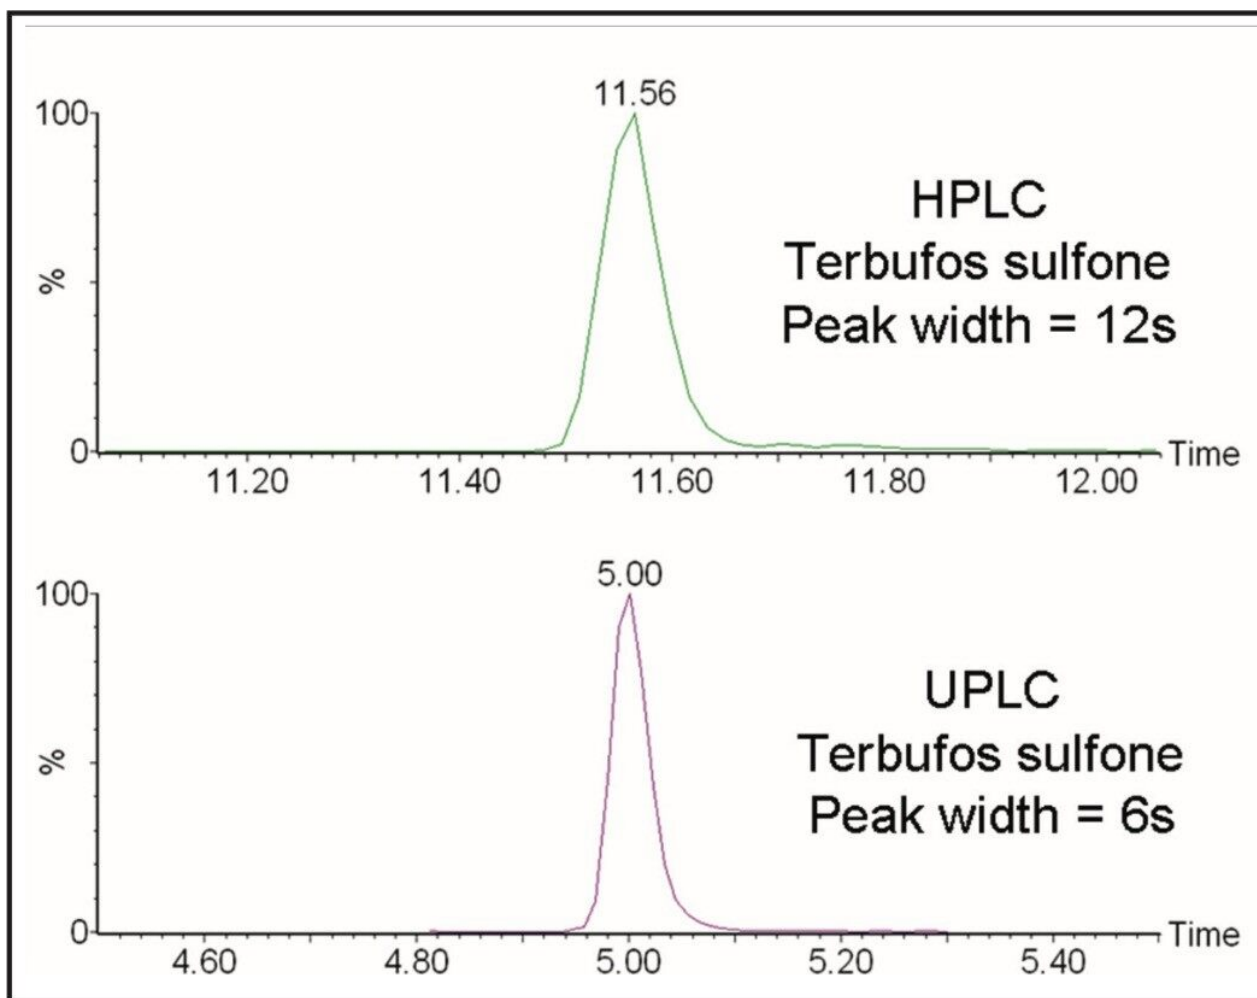


Figure 3. Comparison of peak width for terbufos sulfone from HPLC and UPLC.

Previously, the use of small diameter particle sizes has increased the potential for columns to block but this was proved not to be the case for this type of extract using the UPLC column technology. More than 300 injections of acetonitrile extracts from baby food, made up of 64 solvent injections and 244 matrix injections were analyzed in a single sequence without any significant change in column back pressure, retention time, peak shape, or peak area.

The extraction and analytical methods were further tested for 10 different baby foods ranging from simple, low fat (fruit-based) to complex, high fat (meat-based). The mean recovery, % RSD and ion ratio statistics for each analyte with two determinations in the 10 different baby foods, spiked at 0.001 mg/kg, are listed in Table 7.



<b>Pesticide Residue</b>	<b>Mean Recovery (% RSD)</b>	<b>Ion Ratio (% RSD)</b>
Cadusafos	100 (4)	0.542 (6)
Demeton-s-methyl	102 (5)	0.126 (8)
Demeton-s-methylsulfone	237 (8)	0.396 (9)
Dimethoate	99 (7)	0.767 (12)
Disulfoton	98 (12)	0.078 (22)
Disulfoton sulfone	100 (6)	0.097 (8)
Disulfoton sulfoxide	102 (6)	0.605 (6)
Ethoprophos	101 (5)	0.896 (4)
Fensulfothion	101 (6)	0.940 (6)
Fensulfothion-oxon	101 (5)	0.955 (5)
Fensulfothion-oxon-sulfone	102 (6)	0.896 (4)
Fensulfothion sulfone	102 (7)	0.397 (8)
Omethoate	89 (5)	0.732 (8)
Oxydemeton-s-methyl	104 (5)	0.541 (5)
Terbufos	102 (7)	0.323 (12)
Terbufos sulfone	102 (5)	0.496 (6)
Terbufos sulfoxide	101 (5)	0.363 (4)

Table 7. Mean recovery, % RSD, and ion ratios using UPLC-MS/MS for 0.001 mg/kg recovery samples in 10 different matrices (n = 20).

#### GC-MS/MS

To test the extraction method described, seven recovery experiments were performed in fruit-based and

potato-based baby foods, spiked at 0.001 mg/kg. The mean recovery and relative standard deviation (% RSD) in parenthesis of each analyte are listed in Table 8.

Good recoveries in the range 71–105% with % RSDs of less than 19% were obtained by GC-MS/MS for all the pesticides spiked at the 0.001 mg/kg levels in two different baby foods.

<b>Pesticide Residue</b>	<b>Fruit</b>	<b>Potato</b>
Aldrin	84 (10)	77 (7)
Cadusafos	86 (12)	91 (2)
Dieldrin	93 (6)	84 (7)
Dimethoate	93 (8)	91 (6)
Endrin	100 (8)	89 (8)
Ethoprophos	82 (11)	86 (10)
Fipronil	97 (10)	105 (4)
Fipronil de-sulfinyl	99 (9)	102 (6)
Heptachlor	102 (5)	87 (8)
Heptachlor epoxide	102 (6)	93 (7)
Hexachlorobenzene	77 (7)	71 (4)
Nitrofen	102 (5)	97 (6)
Omethoate	83 (19)	78 (13)

*Table 8. Mean recovery and % RSD using GC-MS/MS for 0.001 mg/kg recovery samples (n = 7).*

Calibration curves were linear over the range 0.0005 - 0.0100 µg/mL with correlation coefficients greater than 0.99 for all analytes using GC-MS/MS.

With GC-MS/MS, all pesticides could be confirmed at the 0.001 mg/kg level with a signal-to-noise (S/N)

ratio of at least 3:1. Table 9 shows the ion ratio statistics for 14 recovery experiments across the two matrices. The % RSDs indicate good repeatability within the tolerances specified in the EU legislation.

<b>Pesticide Residue</b>	<b>Fruit and Potato (% RSD)</b>	<b>2002/657/EC5</b>
Aldrin	0.645 (10)	20
Cadusafos	0.364 (10)	25
Dieldrin	0.621 (10)	20
Dimethoate	0.240 (20)	25
Endrin	0.650 (9)	20
Ethoprophos	0.992 (7)	20
Fipronil	0.784 (8)	20
Fipronil de-sulfinyl	0.834 (9)	20
Heptachlor	0.593 (9)	20
Heptachlor epoxide	0.781 (14)	20
Hexachlorobenzene	0.674 (6)	20
Nitrofen	0.846 (11)	20
Omethoate	0.518 (10)	20

*Table 9. Ion ratios using GC-MS/MS for 0.001 mg/kg recovery samples in two different matrices (n = 14).*

The robustness of the Quattro micro GC was investigated with this type of extract. Fifty-two injections of acetonitrile extracts from baby food were analyzed in a single sequence without any significant change in the response observed. Figure 5 demonstrates the peak area stability of the internal standard,  $\delta$ -HCH. The % RSD across the batch was 5.0%.

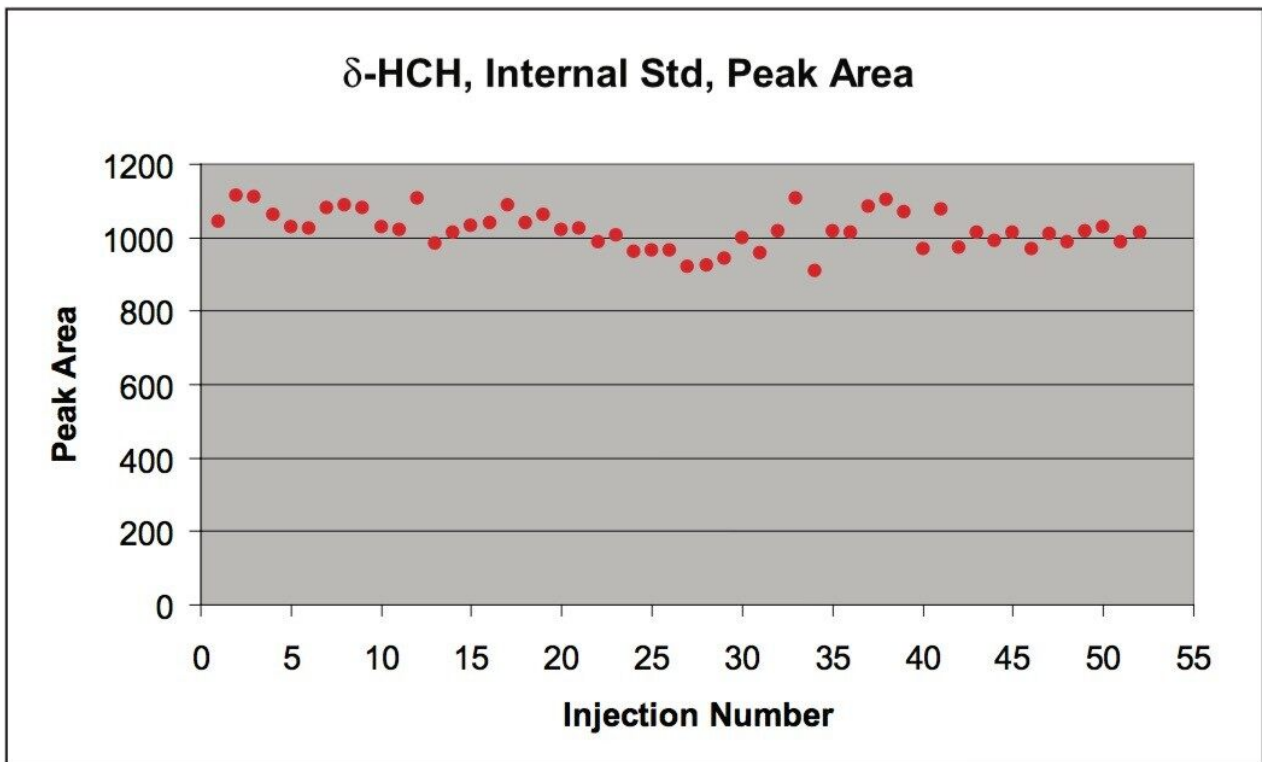


Figure 5. δ-HCH response maintained over 52 matrix injections.

## Conclusion

LC and GC methods have been described for the determination and confirmation of 25 priority pesticide residues and transformation products in different baby foods.

The extraction method yielded very good recoveries and precision at the low concentration levels required by legislation in a range of complex food commodities.

UPLC-MS/MS allows improved confirmation of disulfoton and terbufos in the baby foods tested, due to the enhancement of response and S/N. Another significant advantage with the use of UPLC is the speed of the chromatographic separation, with a 2.5 times increase in throughput compared to HPLC.

The sensitivity offered by ACQUITY UPLC with Quattro Premier XE for the LC amenable compounds and Quattro micro GC for the GC amenable compounds allows the method to meet the challenges set by the EU Baby Food Directive 2003/13/EC.<sup>1</sup>

---

## References

1. Commission Directive 2003/13/EC amending Directive 96/5/EC on processed cereal-based foods and baby foods for infants and young children, Off J of the European Communities No. L41/33.
2. M Anastassiades, S Lehotay, D Stajnbaher, F Schenck, *J. AOAC Int.* 86 (2) (2003) 412.
3. S J Lehotay, K Ma\_tovska, S J Yun, *J AOAC Int.* 88 (2) (2005) 630.
4. M E Swartz, LC GC Europe, Separation Science, June (2005) 5.
5. Commission Directive 2002/657/EC implementing Council Directive 96/23/ EC concerning the performance of analytical methods and the interpretation of results, Off J of the European Communities No. L221/8.

---

## Featured Products

Alliance HPLC System <<https://www.waters.com/534293>>

ACQUITY UPLC System <<https://www.waters.com/514207>>

MassLynx MS Software <<https://www.waters.com/513662>>

TargetLynx <<https://www.waters.com/513791>>

720001436, September 2007