


Nota applicativa

Analysis of Nitrofurantolone Veterinary Drug Residues Using ACQUITY UPLC and Quattro Premier XE

James Morphet, Peter Hancock

Waters Corporation

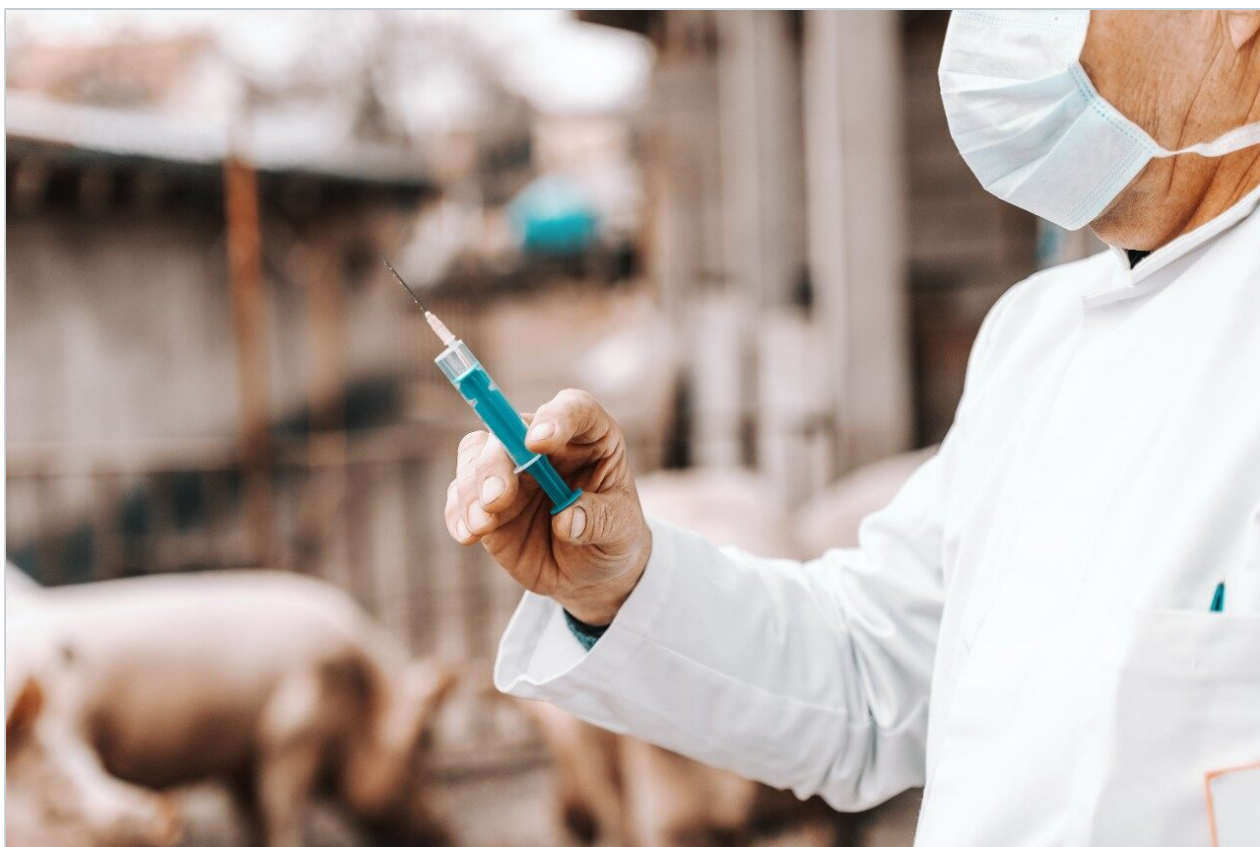

Abstract

This application note describes the transfer of existing HPLC methods to the Waters ACQUITY UPLC System. Standard solutions were used to assess chromatography as there will not be changes to the extraction of metabolites from edible tissues¹ or honey.²

Introduction

The four drugs furazolidone, furaltadone, nitrofurazone, and nitrofurantoin are veterinary drugs that belong to the family of nitrofuran antibiotics and are banned in meat destined for human consumption.³

The four drugs are readily metabolized in livestock to undetectable levels, metabolizing to AOZ, AMOZ, SCA, and AHD, respectively. Their metabolites are more persistent in edible tissues and these can be used to detect use of the parent drug. Proportions of these metabolites exist as protein adducts and the established method of analysis contains acid hydrolysis and derivatisation steps prior to extraction.⁴

This method transfer will determine the suitability of UPLC for the determination of these residues. Previous methods¹ have employed HPLC-MS/MS using a Waters Alliance 2795 System with a Waters Quattro Premier XE Mass Spectrometer. The ACQUITY UPLC has been designed to significantly reduce run times using novel column chemistries. ACQUITY UPLC also gives advantages over regular HPLC in sensitivity, specificity, accuracy, and resolution.



ACQUITY UPLC System coupled with a Quattro Premier XE Mass Spectrometer

Experimental

A solution containing the four derivatized metabolites and their deuterated internal standards, 2-NPAMOZ-D₅, 2-NP-SCA-¹³C₁ ¹⁵N₂, and 2-NP-AHD¹³C₃ was produced at a concentration of 8 ng/mL (equivalent to 2 ppb in animal tissue) in 1:4 methanol: water (v/v). This solution was further diluted to 4, 2, 0.4, and 0.2 ng/mL (equivalent to 1, 0.5, 0.1, and 0.05 ppb in extracted samples¹).

A standard curve was created for all compounds and the chromatography was assessed for each compound at each level. All concentrations reported in this technical note refer to the derivitized metabolite.

Mobile phase A was 1:4 methanol: water (v/v) + 0.5 mM ammonium acetate. Mobile phase B was 9:1

methanol: water (v/v) + 0.5 mM ammonium acetate. The column used was an ACQUITY UPLC BEH C₁₈ 1.7 μm 2.1 x 100 mm. A 50 μL injection was used with a flow rate of 0.45 mL/min.

The gradient used is described below:

0.00 min 5% mobile phase B (hold 0.2 min)

2.00 min 50% mobile phase B

2.02 min 100% mobile phase B (hold 1.1 min)

Total run time was 4.00 minutes.

The Quattro Premier XE was set up in positive ion mode using an electrospray source. All compounds were optimized and two Multiple Reaction Monitoring (MRM) transitions were obtained for each derivatized metabolite and one for each internal standard. Two MRM transitions were monitored for each derivatized metabolite in accordance with European Union guidelines.⁵ The primary transition is used for quantification and the secondary transition is used for conformation purposes. These MRM transitions are listed in Table 1 along with their respective cone voltages and collision energies.

Metabolite	MRM Transition	Cone voltage (V)	Collision energy (eV)
2-NP-AOZ	236.1>103.9	30	22
	236.1>134.0	30	15
2-NP-AMOZ	335.5>100.0	32	26
	335.5>291.3	32	12
2-NP-SCA	209.1>166.0	24	8
	209.1>192.1	24	10
2-NP-AHD	249.5>133.9	30	11
	249.5>103.9	30	19
2-NP-AOZ-D₄	240.1>134.4	30	13
2-NP-AMOZ-D₅	340.2>296.4	30	12
2-NP-SCA-¹³C₁ ¹⁵N₂	212.0>168.0	26	9
2-NP-AHD-¹³C₃	252.1>133.9	30	12

Table 1. MRM transitions for the derivatized metabolites and their internal standards.

A dwell time of 0.025 s was chosen for this analysis. This gave approximately 14 points per chromatographic peak.

The following electrospray parameters were used on the Quattro Premier XE:

Capillary voltage:	3 kV
Extractor:	4 V
RF Lens:	0.5 V
Source temperature:	120 °C

Desolvation gas temperature:	400 °C
Desolvation gas (nitrogen):	900 L/hr
Cone gas (nitrogen):	20 L/hr
Collision cell gas (argon):	3.3 10 ⁻³ mBar

Data were acquired with Waters MassLynx Software and processed with Waters TargetLynx Application Manager.

Results and Discussion

Sensitivity was achieved for all components of the derivatized metabolite mixture at 0.4 ng/mL (equivalent to 0.1 ppb). This is ten times below the EU minimum required performance limit (MPRL) guideline.

Figures 1, 2, and 3 show typical chromatography obtained using ACQUITY UPLC. The novel technology offered by UPLC gives the advantage of a run time of four minutes, compared to the traditional HPLC run time of approximately 10 minutes.

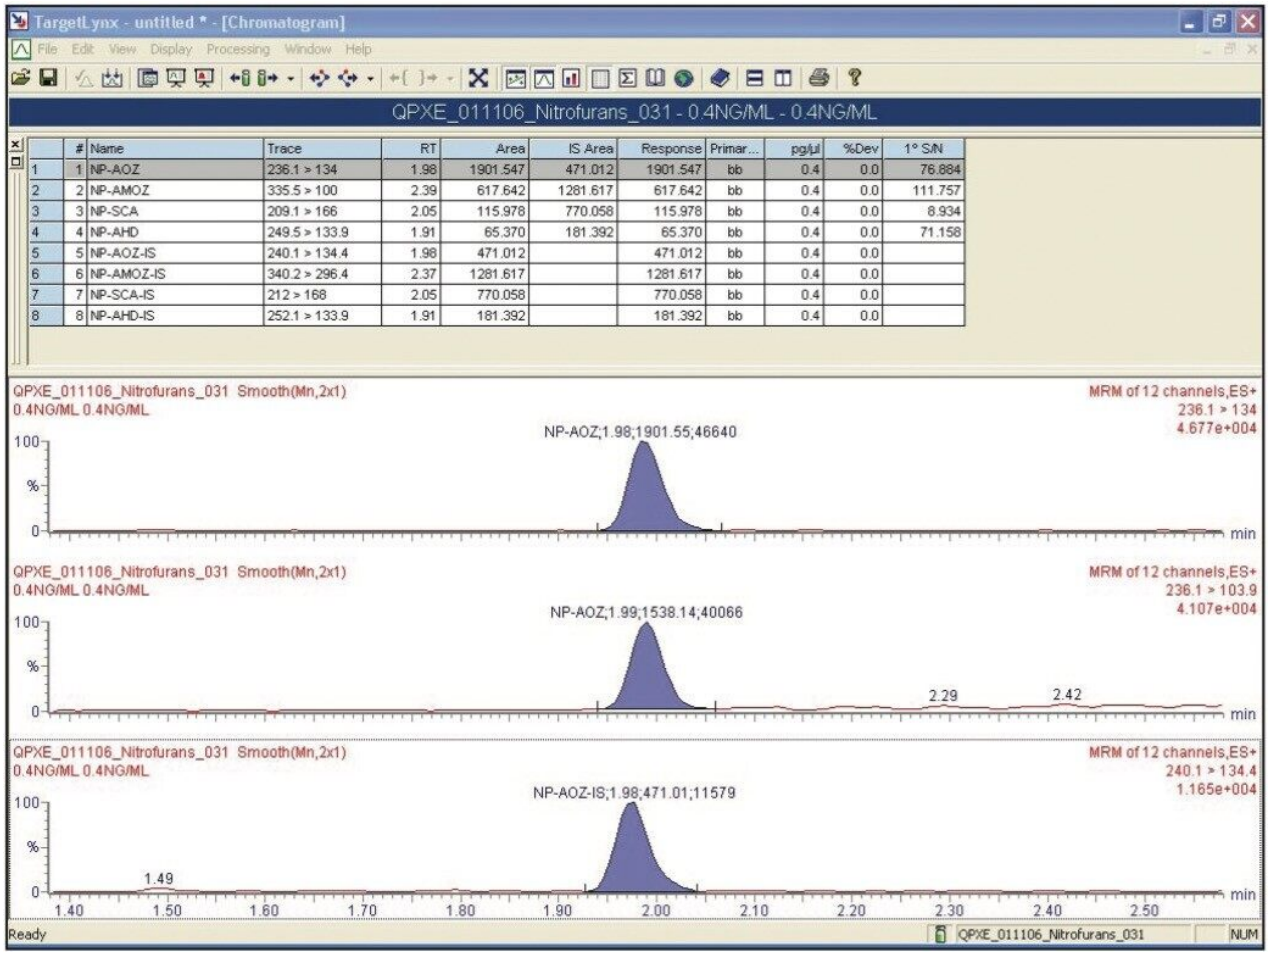


Figure 1. TargetLynx view detailing peak shape for NP-AOZ, response and S:N ratio for all the derivatized metabolites at 0.4 ng/mL (equivalent to 0.1 ppb in animal tissue) – ten times below the MRPL.

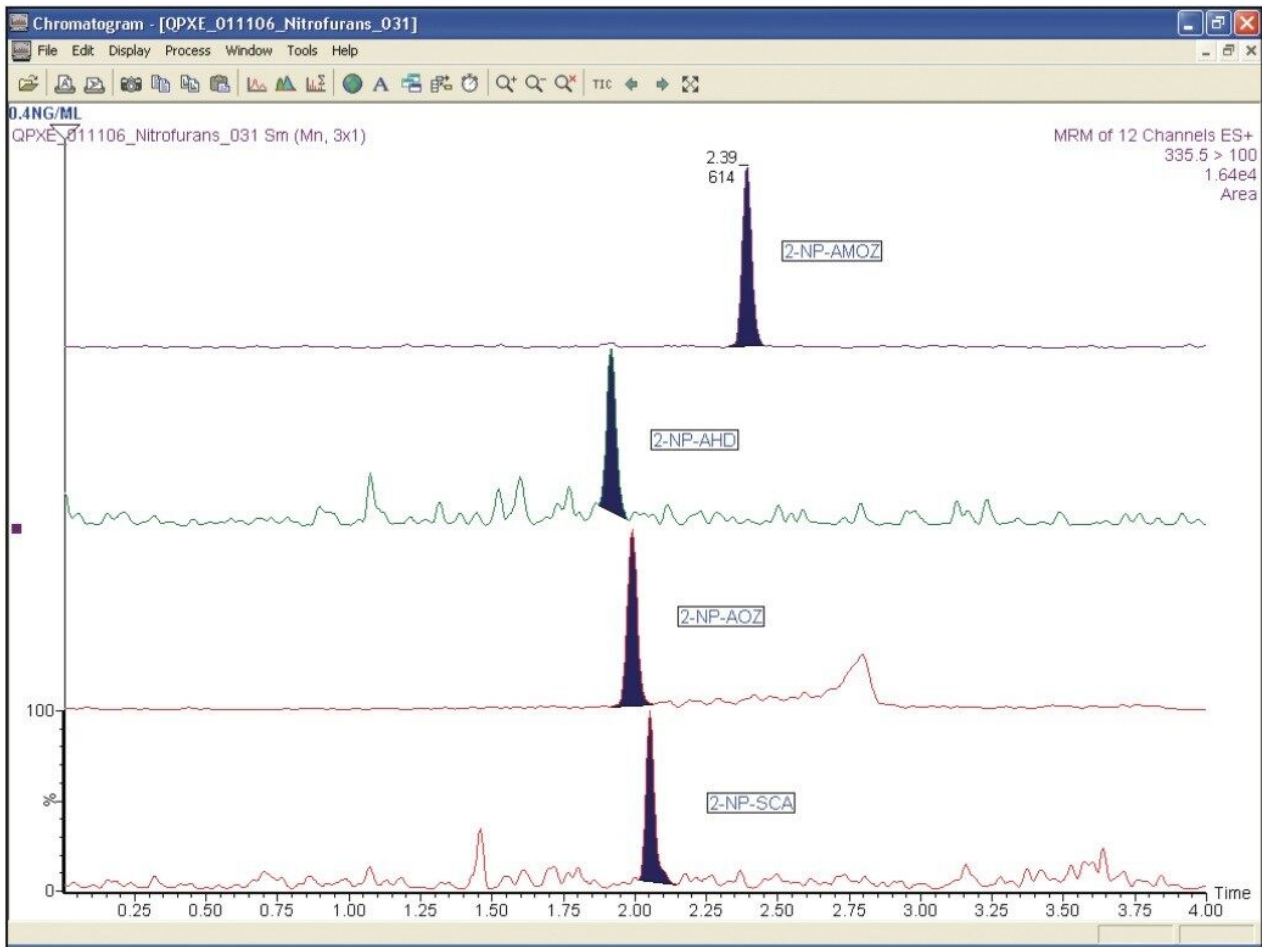


Figure 2. MassLynx screen shot showing chromatography at 0.4 ng/mL (equivalent to 0.1 ppb – ten times below the MRPL) achieved using ACQUITY UPLC.

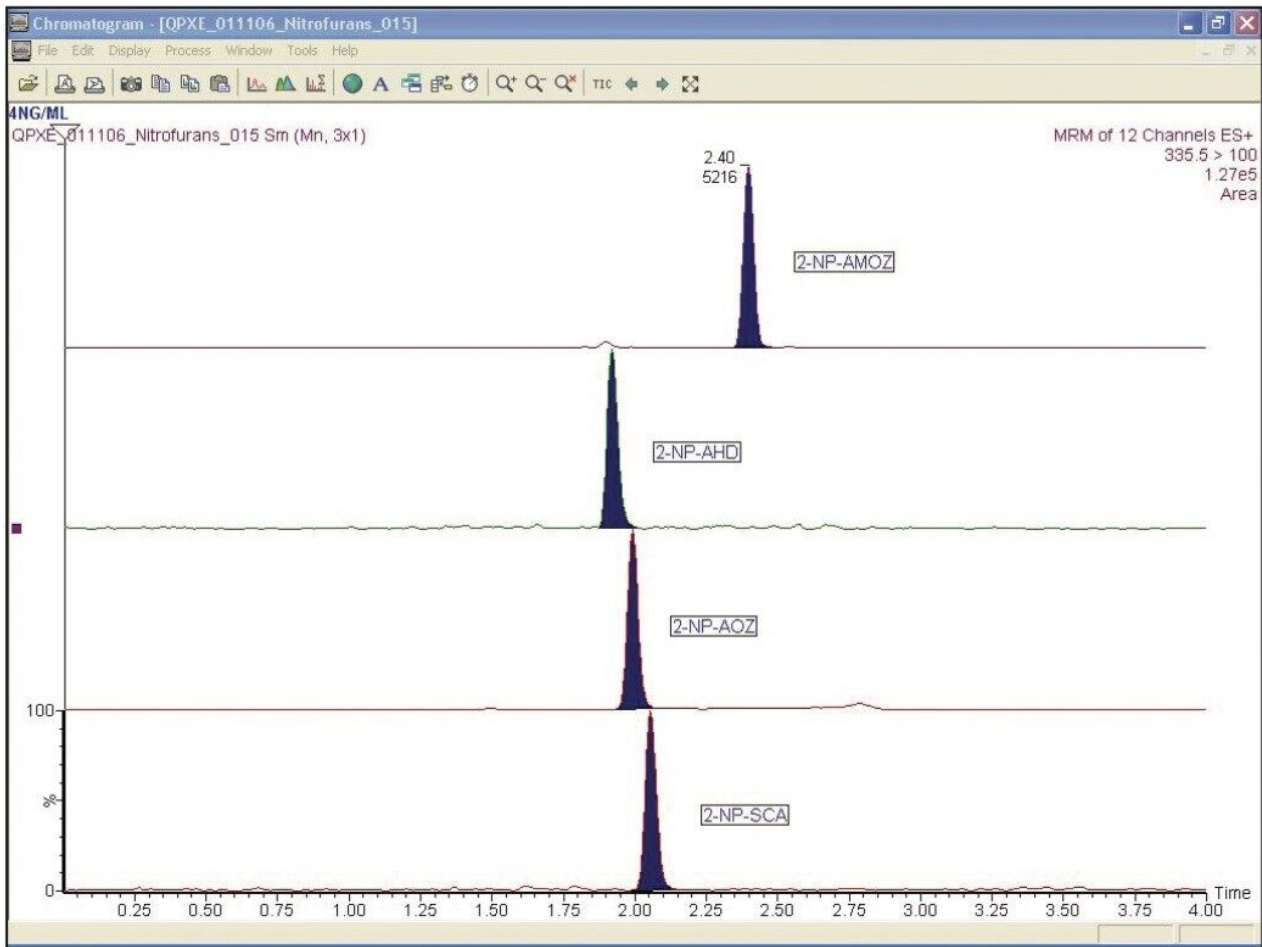


Figure 3. Chromatography at 4 ng/mL- equivalent to 1 ppb (the MPRL) achieved using ACQUITY UPLC.

When assessing the Signal to Noise (S:N) ratio's for all derivatized nitrofurans metabolites it is clear that they have differing response factors. An acceptable limit of detection was allowed to be a S:N ratio of 3:1. All derivatized nitrofurans metabolites have a S:N ratio significantly greater than this value at 0.4 ng/mL (equivalent to 0.1 ppb). Figures 2 and 3 show the chromatographic separation of the four derivatized nitrofurans metabolites with a four minute run time.

Conclusion

The established HPLC method for the determination of nitrofurans veterinary drug residues has been successfully transferred to a UPLC coupled to a Quattro Premier XE Mass Spectrometer. The new UPLC

method provides a two fold increase in the speed of separation over the HPLC method with excellent sensitivity that allows detection at ten times below the EU minimum required performance limit (MPRL) guideline.

References

1. Determination of Nitrofurans Veterinary Drug Residues, Waters Application Note No. 720000847EN <<https://www.waters.com/webassets/cms/library/docs/720000847en.pdf>> .
2. LC-MS/MS Determination of Nitrofurans Metabolite Residues in Honey, Waters Application Note No. 720001034EN <<https://www.waters.com/webassets/cms/library/docs/oasis203.pdf>> .
3. Commission Regulation (EC) 1442/95, Official J. European Communities, No. L143/26.
4. *Analytica Chimica Acta*, 483 (2003) 91–98.
5. Commission Directive 2002/657/EC, Off. J. of the European Communities No. L221/8.

Featured Products

[ACQUITY UPLC System <https://www.waters.com/514207>](https://www.waters.com/514207)

[MassLynx MS Software <https://www.waters.com/513662>](https://www.waters.com/513662)

[TargetLynx <https://www.waters.com/513791>](https://www.waters.com/513791)

720001951, September 2007

© 2021 Waters Corporation. All Rights Reserved.