

Note d'application

## High Definition Mass Spectrometry as a Tool for Structural Investigation of High $m/z$ Ion Species

---

Iain Campuzano, Kevin Giles

Waters Corporation

This is an Application Brief and does not contain a detailed Experimental section.

---

### Abstract

Here we present the use of high-efficiency IMS (Triwave technology) on a SYNAPT High Definition Mass Spectrometry (HDMS) System for analysis of high  $m/z$  caesium iodide clusters over the  $m/z$  range 1,000–20,000. This demonstrates the utility of the SYNAPT HDMS System for the mass measurement of high  $m/z$  species, such as in the analysis of non-covalent protein complexes.

---

### Introduction

Over the past 10 years, interest in high mass non-covalent analysis has increased due to the ability of the current mass spectrometers and electrospray sources to preserve the non-covalent interactions, allowing one to analyze compounds in their native conformation and stoichiometry.<sup>1</sup> The transfer of non-covalently associated complexes from solution to the gas phase using electrospray ionization generally results in the formation of ions possessing

---

relatively few charges. As a result, these species appear high on the  $m/z$  scale, making Time-of-Flight mass spectrometry ideal for their mass analysis. The utility of ion mobility spectrometry (IMS) in probing the structures of relatively large complexes has been highlighted previously.<sup>1</sup>

Here we present the use of high-efficiency IMS (Triwave technology) on a SYNAPT High Definition Mass Spectrometry (HDMS) System for analysis of high  $m/z$  caesium iodide clusters over the  $m/z$  range 1,000–20,000. This demonstrates the utility of the SYNAPT HDMS System for the mass measurement of high  $m/z$  species, such as in the analysis of non-covalent protein complexes.

---


## Experimental

The instrument used in this study was a SYNAPT HDMS System, which combines high-efficiency ion mobility based measurements and separations with a hybrid quadrupole orthogonal acceleration Time-of-Flight (oa-ToF) mass spectrometer, Figure 1.<sup>2</sup> Samples were introduced with a borosilcate-glass nano electrospray-spray tip and sampled into the vacuum system. The ions pass through a quadrupole mass filter to the enabling Triwave device. Triwave consists of three travelling wave (T-Wave) ion guides. The TRAP T-Wave accumulates ions (with high efficiency), after which these ions are released as discrete packets into the IMS T-Wave, where the ion mobility separation of ions is performed. The TRANSFER T-Wave is used to deliver the ion mobility-separated ions into the oa-ToF analyzer. Each IMS separation was 51 ms long and the ions were released from the TRAP T-wave in 500  $\mu$ s wide packets. The gas pressure in the TRAP and TRANSFER T-Wave regions was 0.07 mbar (Argon) and the pressure in the IMS T-Wave was 0.5 mbar (Nitrogen). The traveling wave used in the IMS T-Wave for ion mobility separation was operated at a velocity of 250 m/sec. The wave amplitude was ramped from 0 to 30 V over the period of the mobility separation for optimum performance over the large  $m/z$  range used ( $m/z$  1,000 to 32,000).

## MS Conditions

MS system:	SYNAPT HDMS System
Ionization mode:	nanoESI positive

Capillary voltage:	1000 V
Cone voltage:	150 V
Source temp.:	40 °C
Acquisition range:	1,000 to 32,000 $m/z$
IMS T-wave ramp:	0 to 3.0 V over IMS experiment
IMS T-wave speed:	250 m/sec
IMS pressure:	0.5 mbar (nitrogen)

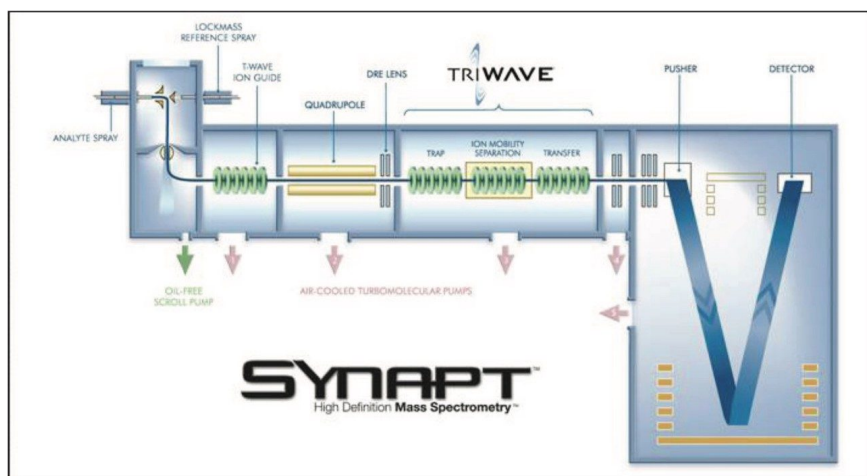

*Figure 1. Schematic of the SYNAPT HDMS System.*

## Results and Discussion

Upon MS acquisition of a concentrated caesium iodide solution, intense ion clusters can be observed as high as

$m/z$  20,000, with each cluster's composition based on the formula  $Cs(n+1)In$ . From the mass spectrum generated it is evident that a number of overlapping series, differing in charge state and intensity profile, are present over the  $m/z$  scale (Figure 2). However, the HDMS (IMS/MS) analysis clearly illustrates discrete distributions, which are related by their  $m/z$  and drift-time, as shown in Figure 3.

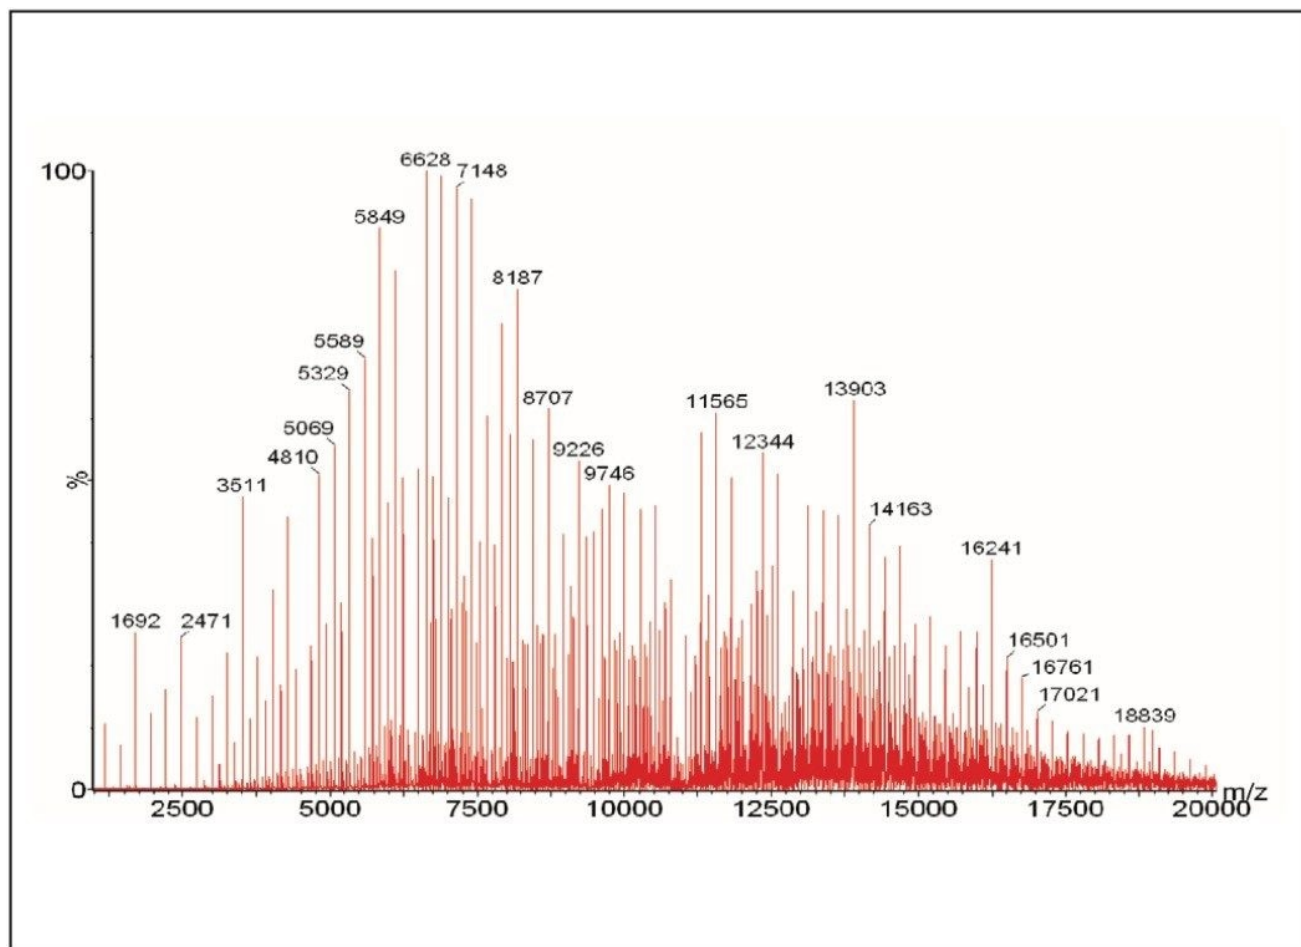


Figure 2. Mass spectrum of CsI ( $m/z$  1,000 to 20,000).

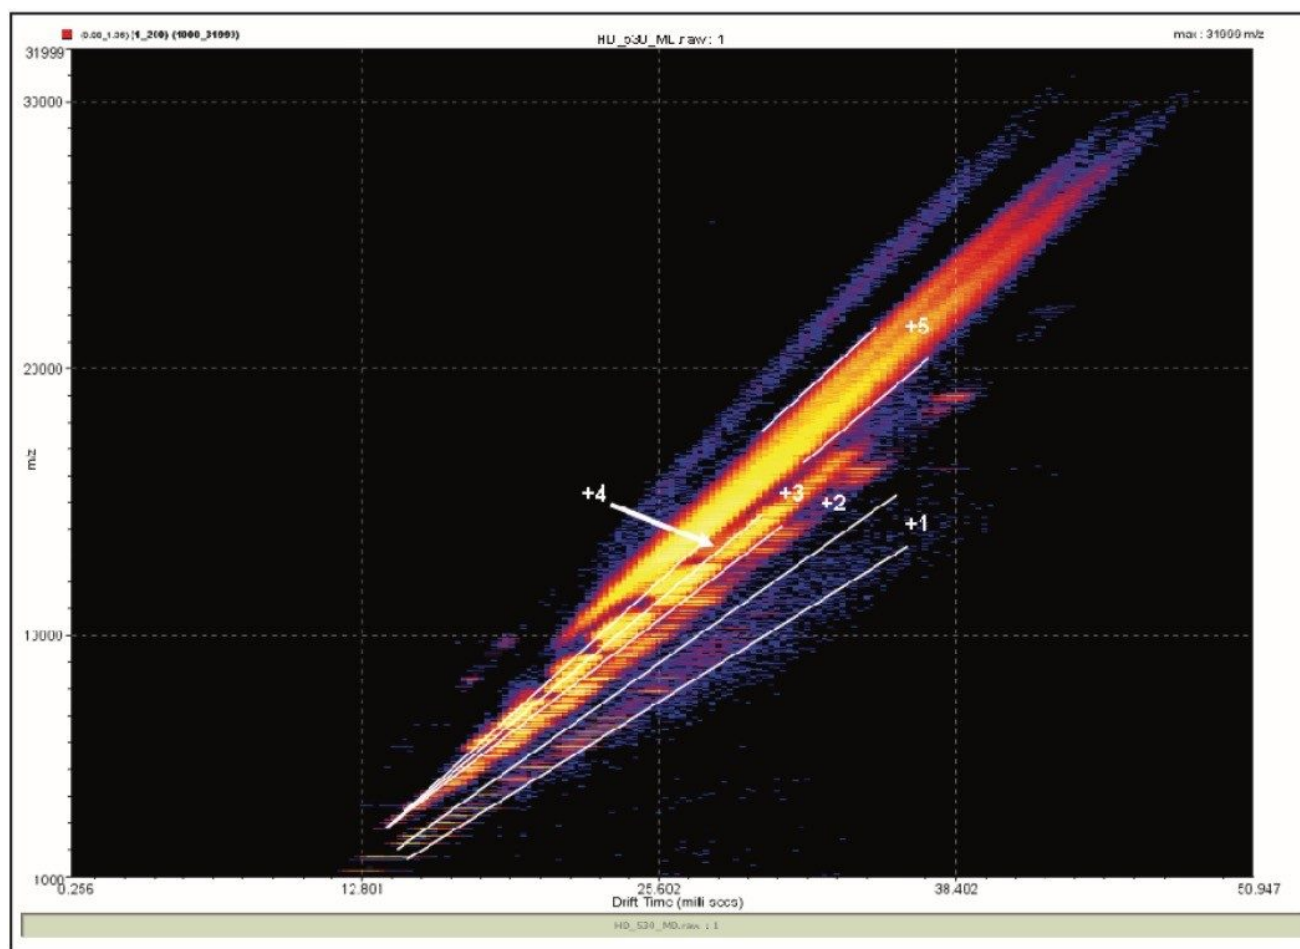


Figure 3. HDMS analysis: Drift-time vs  $m/z$  plot of CsI ( $m/z$  1,000 to 32,000).

The drift-times of the cluster ions seem to increase monotonically with increasing  $m/z$  values for the different charge state species, although with increasing charge state series up to +4, distinct  $m/z$  stability regions become clear, as shown in Figure 4.

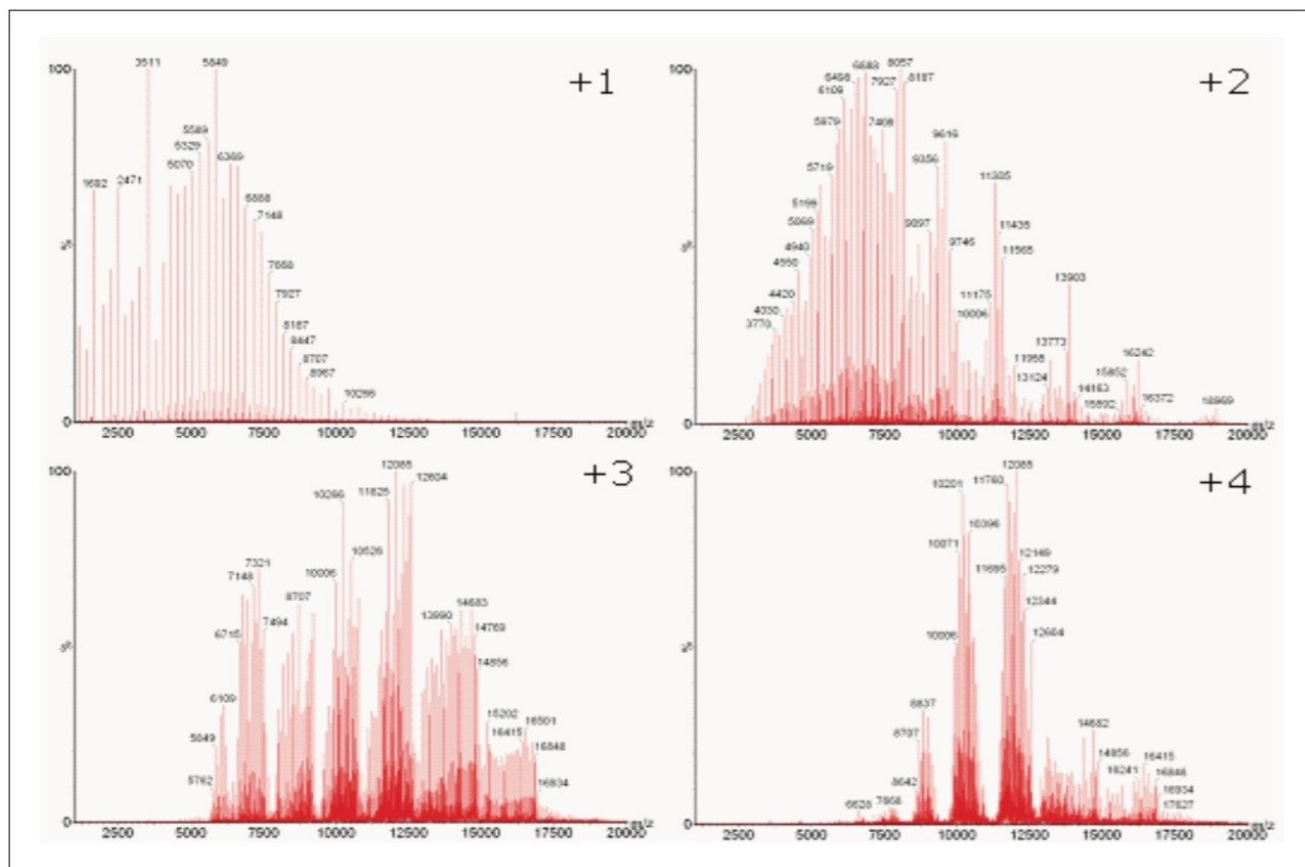


Figure 4. Charge state distributions of Csl.

## Conclusion

- HDMS provides greater definition of even relatively simple samples, such as inorganic Csl clusters
- High mass analysis of Csl clusters up to  $m/z$  20,000 has been shown
- Csl clusters have been successfully separated into five charge states series, demonstrating the ability of HDMS (high-efficiency IMS combined with oa-ToF mass spectrometry) for differentiating high mw species based on their mobility
- Csl can be used to tune, optimize, and calibrate the SYNAPT HDMS System over a wide  $m/z$  range prior to high mass acquisitions being carried out

---

## References

1. Ruotolo, Giles, Campuzano, Sandercock, Bateman & Robinson. *Science*. 310 (2005) 1658–1661.
2. Pringle, Giles, Wildgoose, Williams, Slade, Thalassinou, Bateman, Bowers, Scrivens. *Int. J. Mass Spectrom.*, 261 (2007) 1–12.

---

## Featured Products

TriWave <<https://www.waters.com/134663660>>

720002632, May 2008

© 2022 Waters Corporation. All Rights Reserved.

[Terms of Use](#)

[Privacy](#)

[Trademarks](#)

[Sitemap](#)

[Careers](#)

[Cookies](#)

[Préférences de cookies](#)