

ACQUITY UPLC Analysis of Thiourea

Waters Corporation




This is an Application Brief and does not contain a detailed Experimental section.

Abstract

This application brief demonstrates the analysis of Thiourea.

Introduction

Structure

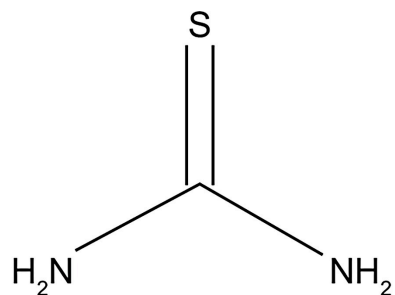

Thiourea


Experimental

Test Conditions

Column:	ACQUITY UPLC BEH Amide, 2.1 x 150 mm, 1.7 μ m
Part Number:	186004802
Isocratic Mobile Phase:	95/2.5/2.5 MeCN/IPA/H ₂ O with 10 mM CH ₃ COONH ₄ and 0.01% NH ₄ OH, pH 9.0
Flow Rate:	0.2 mL/min
Injection Volume:	5.0 μ L (PLNO)
Sample Concentration:	10 μ g/mL
Sample Diluent:	75/25 MeCN/MeOH with 0.2% HCOOH

Column Temperature:	25 °C
Weak Needle Wash:	95/5 MeCN/H ₂ O
Detection:	UV @ 245 nm
Sampling Rate:	20 points/sec
Filter Time Constant:	0.2
Instrument:	Waters ACQUITY UPLC with ACQUITY UPLC PDA Detector

Results and Discussion

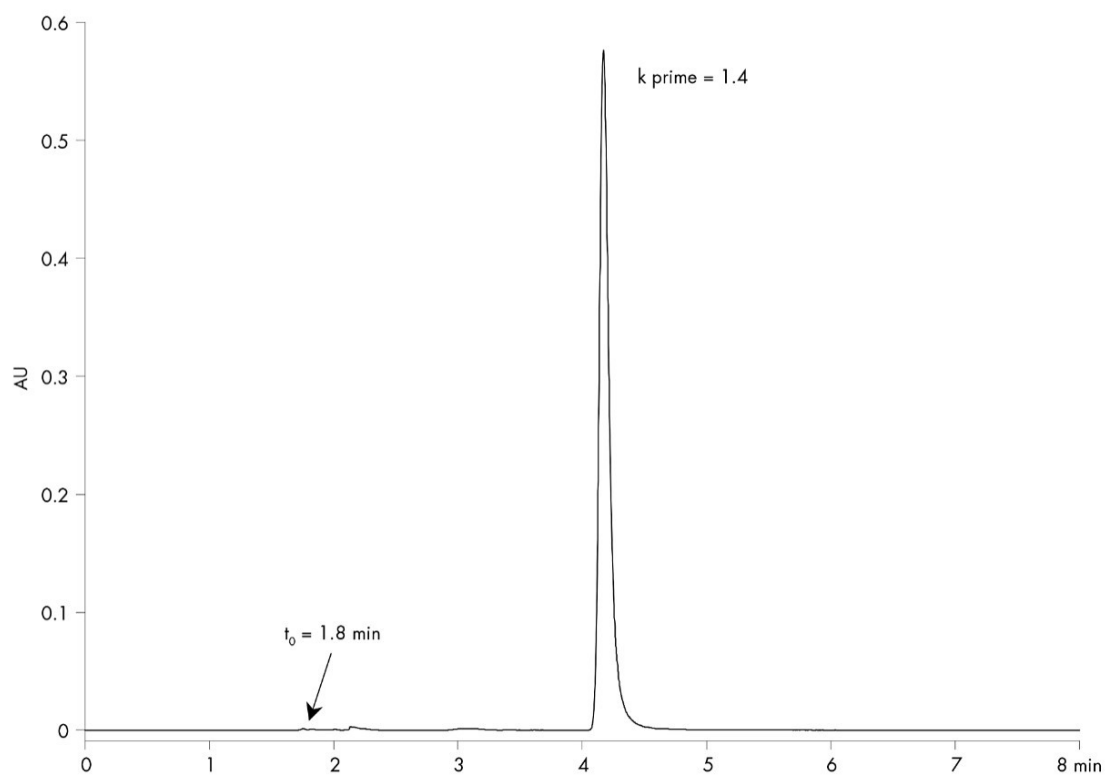

Featured Products

- [ACQUITY UPLC System <https://www.waters.com/514207>](https://www.waters.com/514207)
- [ACQUITY UPLC PDA Detector <https://www.waters.com/514225>](https://www.waters.com/514225)

WA60095, June 2009



©2019 Waters Corporation. All Rights Reserved.