

Application Note

ACQUITY UPLC Analysis of Histidine Dipeptides

Waters Corporation

This is an Application Brief and does not contain a detailed Experimental section.


Abstract

This application highlights the analysis of Histidine Dipeptides on ACQUITY UPLC BEH Amide Columns.


Introduction

The compounds used in this study are:


1. Creatinine (1 µg/mL)
 2. Creatine (5 µg/mL)
 3. Anserine (5 µg/mL)
 4. Canosine (5 µg/mL)
-

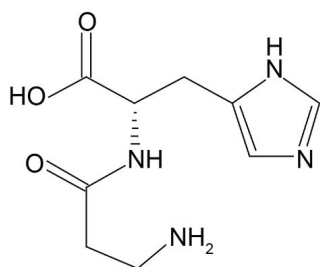


Carnosine

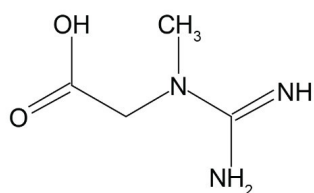

Creatine



Creatinine

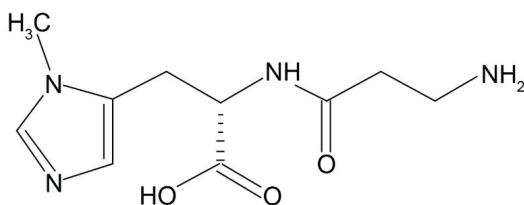

Anserine

Experimental

Chromatographic Conditions

Column:	ACQUITY UPLC BEH HILIC, 2.1 x 50 mm, 1.7 μm
Part Number:	186004800
Mobile Phase A:	50/50 MeCN/H ₂ O with 10 mM CH ₃ COONH ₄ and 0.04 % NH ₄ OH, pH 9.0
Mobile Phase B:	95/5 MeCN/H ₂ O with 10 mM CH ₃ COONH ₄ and 0.04 % NH ₄ OH, pH 9.0

Flow Rate: 0.5 mL/min

Injection Volume: 5 µL

Sample Diluent: 75/25 MeCN/MeOH

Column Temperature: 30 °C


Weak Needle Wash: 95/5 MeCN/H₂O

Instrument: Waters ACQUITY UPLC with ACQUITY SQD

Gradient

Time (min)	Profile	
	%A	%B
Initial	0.1	99.9
5.00	65.0	35.0
5.01	0.1	99.9
6.00	0.1	99.9

Results and Discussion

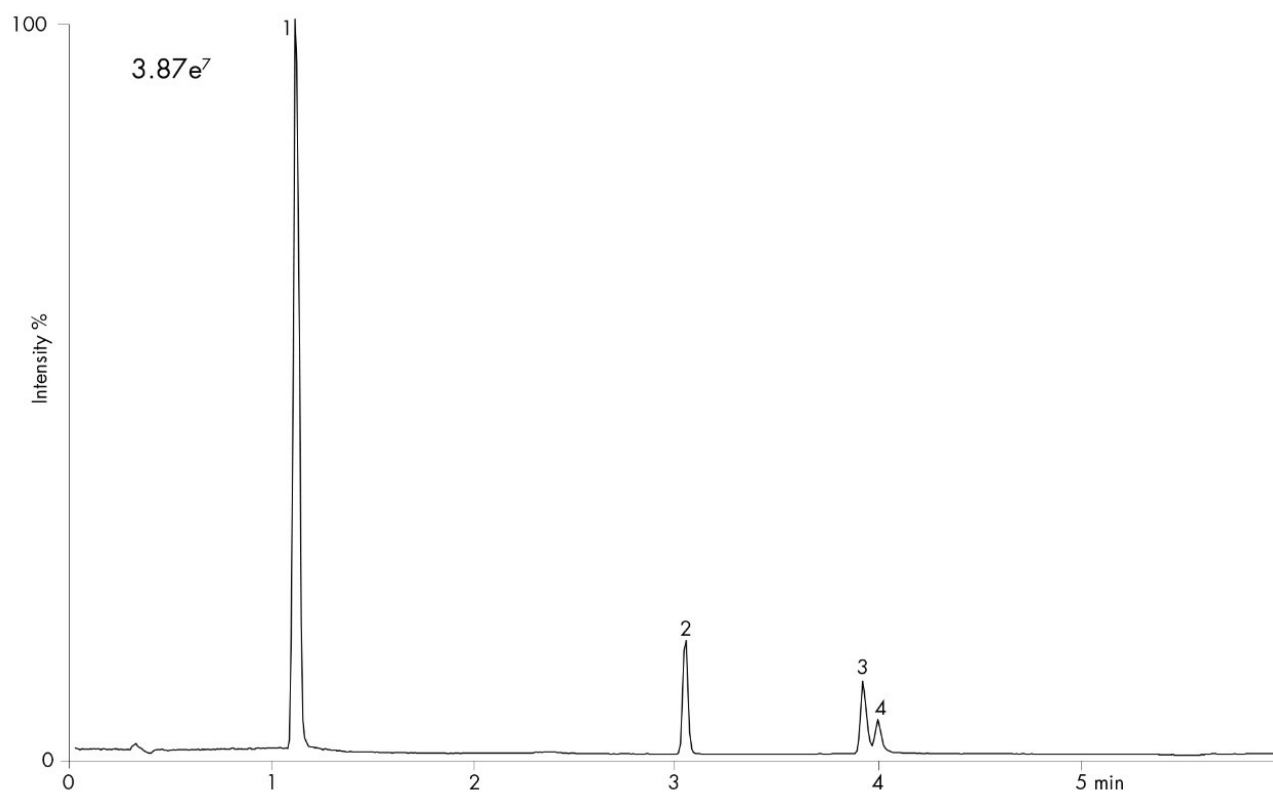

Featured Products

SQ Detector 2 <<https://www.waters.com/134631584>>

WA60103, July 2009

© 2022 Waters Corporation. All Rights Reserved.