

Note d'application

## ACQUITY UPLC Analysis of Allantoin

---

Waters Corporation

This is an Application Brief and does not contain a detailed Experimental section.

---

### Abstract


This application brief highlights the analysis of allantoin on ACQUITY UPLC BEH Amide Columns.

---

### Introduction

---

## Structures

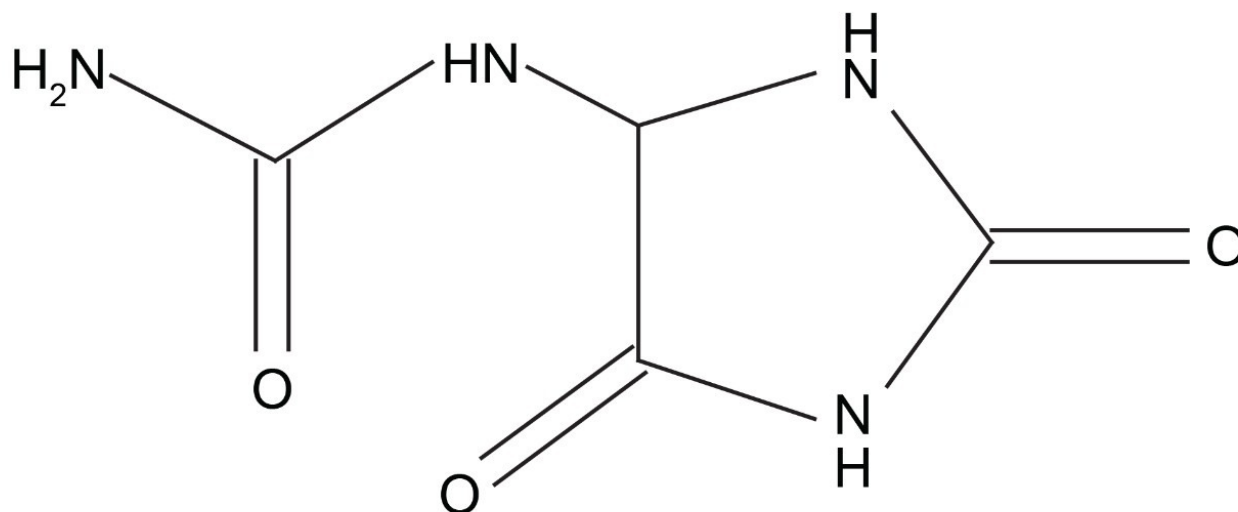

# Allantoin

---

## Experimental

### Test Conditions

Column:	ACQUITY UPLC BEH Amide, 2.1 x 150 mm, 1.7 $\mu$ m
Part Number:	186004802
Isocratic Mobile Phase B:	90/10 MeCN/H <sub>2</sub> O


Flow Rate:	0.2 mL/min
Injection Volume:	5.0 µL (PLNO)
Sample Concentration:	100 µg/mL
Sample Diluent:	90/10 MeCN/H <sub>2</sub> O
Column Temperature:	25 °C
Weak Needle Wash:	95/5 MeCN/H <sub>2</sub> O
Detection:	UV @ 210 nm
Sampling Rate:	20 points/sec
Filter Time Constant:	0.2
Instrument:	Waters ACQUITY UPLC with ACQUITY UPLC PDA Detector

---

## Results and Discussion

The compound used in this study is:

1. Allantoin

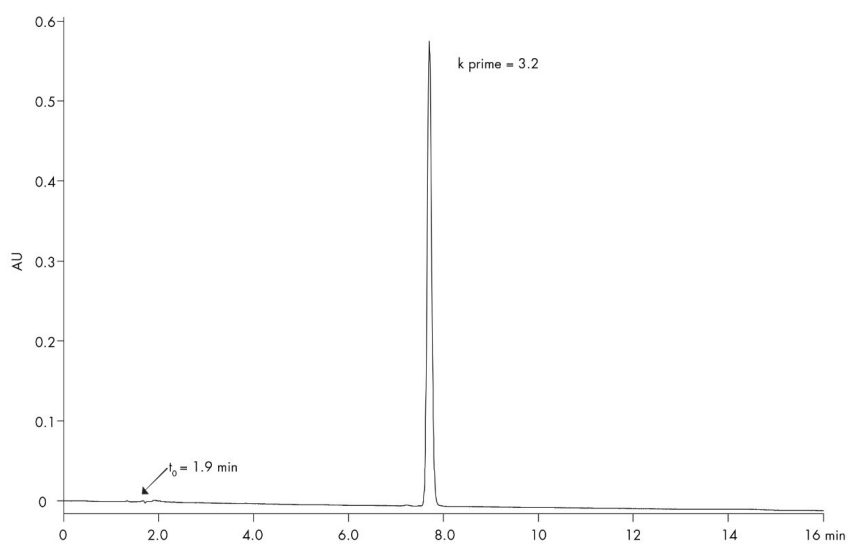

---

## Featured Products

ACQUITY UPLC PDA Detector <<https://www.waters.com/514225>>

WA60107, June 2009

© 2022 Waters Corporation. All Rights Reserved.