

응용 자료

## Analysis of Mono-, Di- and Oligosaccharides Using ACQUITY UPLC BEH Amide Columns

---

Waters Corporation



This is an Application Brief and does not contain a detailed Experimental section.

---

## Abstract

This application brief describes the analysis of Oligosaccharides using ACQUITY UPLC BEH Amide Columns.


---

## Introduction


Compounds used for this study includes:

1. p-Toluamide
2. Fructose
3. Glucose
4. Sucrose
5. Maltose
6. Maltotriose
7. Maltotetraose
8. Maltopentaose
9. Maltohexahose
10. Maltoheptaose


## STRUCTURES

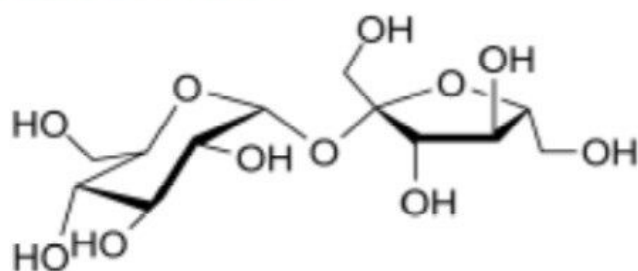


Sucrose

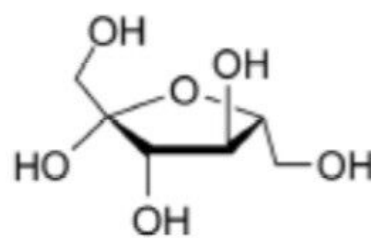


Fructose

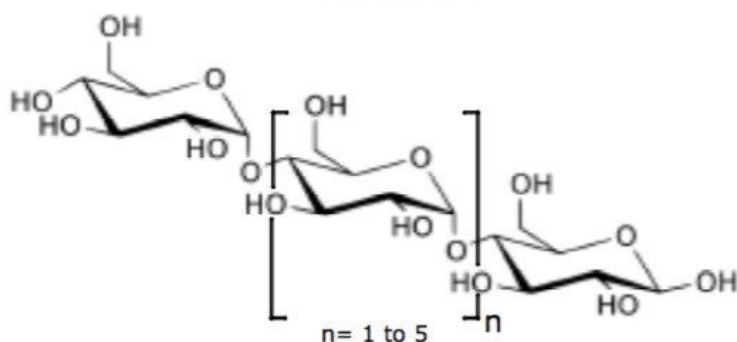


Maltooligosaccharides

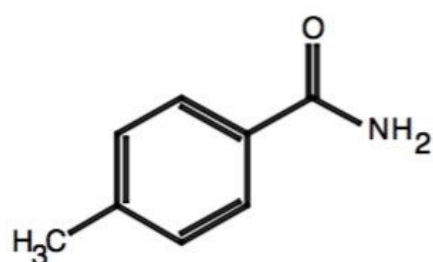

p-Toluamide  
(unretained compound)

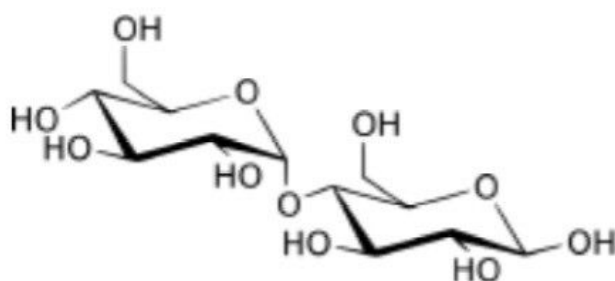

Maltose

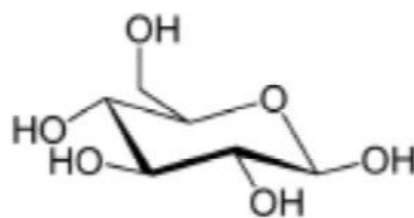

Glucose

---

Experimental

Chromatographic Conditions

Column:	ACQUITY UPLC BEH Amide 2.1 x 50 mm, 1.7 $\mu$ m
Part Number:	186004800
Mobile Phase A:	80/20 MeCN/H <sub>2</sub> O with 0.05% triethylamine [TEA]
Mobile Phase B:	30/70 MeCN/H <sub>2</sub> O with 0.05% triethylamine [TEA]
Flow Rate:	0.17 mL/min
Gradient:	5 minute gradient, 80%-50% MeCN
Injection Volume:	0.7 $\mu$ L (PLNO)
Sample Concentration:	1 mg/mL each
Sample Diluent:	50/50 MeCN/H <sub>2</sub> O
Column Temperature:	35 $^{\circ}$ C
Strong Needle Wash:	20/80 MeCN/H <sub>2</sub> O (800 $\mu$ L)
Weak Needle Wash:	75/25 MeCN/H <sub>2</sub> O (500 $\mu$ L)
Seal Wash:	50/50 MeCN/H <sub>2</sub> O
Instrument:	Waters ACQUITY UPLC with ELSD

### Gradient:

Time (min)	%A	%B
0.00	100.00	0.00


Time (min)	%A	%B
5.00	40.00	60.00
5.01	100.00	0.00
15.00	100.00	0.00

## ELSD Conditions

Gain:	200
Pressure:	40 psi
Drift Tube Temperature:	40 °C
Nebulizer:	Cooling
Data Rate:	10 pps
Filter Time Constant:	Normal

---

## Results and Discussion

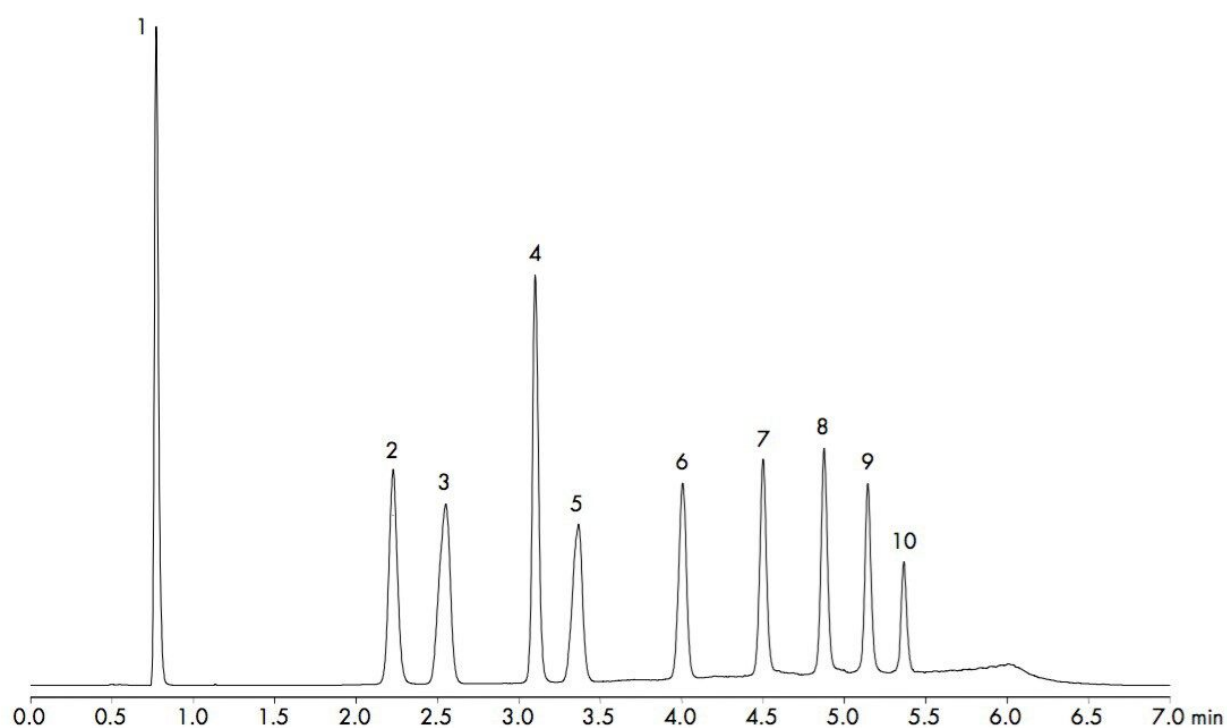

---

## Featured Products

ACQUITY UPLC System <<https://www.waters.com/514207>>

ACQUITY UPLC ELS Detector <<https://www.waters.com/514219>>

WA60110, October 2009