Waters[™]

Note d'application

Analysis of Food Sugars/Saccharides in Beer Using ACQUITY UPLC BEH Amide Columns

Waters Corporation


This is an Application Brief and does not contain a detailed Experimental section.

Abstract

This application brief highlights the analysis of food sugars/saccharides in beer using ACQUITY UPLC BEH Amide Columns.

Introduction

Structures

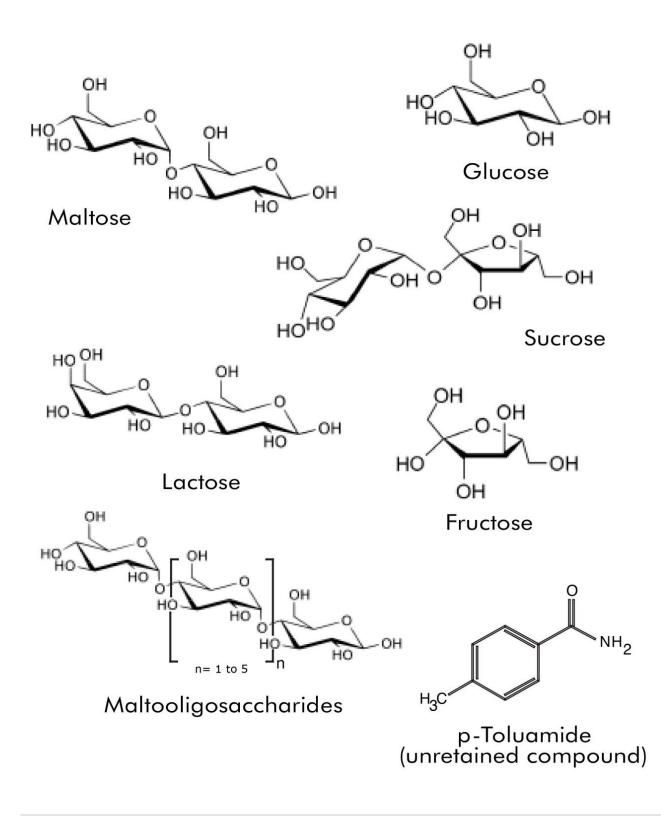

Experimental

Chromatographic Conditions

| Column: | ACQUITY UPLC BEH Amide 2.1 x 100 mm, 1.7 μm |
|-----------------------|---|
| Part Number: | 186004801 |
| Mobile Phase A: | 80/20 MeCN/H ₂ O with 0.2% triethylamine [TEA] |
| Mobile Phase B: | 30/70 MeCN/H ₂ O with 0.2% triethylamine [TEA] |
| Flow Rate: | 0.13 mL/min |
| Gradient: | 10 minute gradient, 80%-50% MeCN (w/0.2% TEA) with 25 minute re-equilibration |
| Injection Volume: | 1.3 µL (PLNO) |
| Sample Concentration: | Standards at 1mg/mL, beer at 100% (No dilution) |
| Sample Diluent: | 50/50 MeCN/H ₂ O |
| Column Temperature: | 35 °C |
| Strong Needle Wash: | 20/80 MeCN/H ₂ O (800 µL) |

| Weak Needle Wash: | 75/25 MeCN/H ₂ O (500 µL) |
|-------------------|--------------------------------------|
| Seal Wash: | 50/50 MeCN/H ₂ O |
| Instrument: | Waters ACQUITY UPLC with ELSD |

Gradient

| Time | Profile | |
|-------|---------|-------|
| (min) | %A | %B |
| 0.00 | 90.00 | 10.00 |
| 10.00 | 30.00 | 70.00 |
| 10.01 | 90.00 | 10.00 |
| 35.00 | 90.00 | 10.00 |

ELSD Conditions

Gain:

200

Pressure:


40 psi

| Drift Tube Temperature: | 40 °C |
|-------------------------|---------|
| Nebulizer: | Cooling |
| Data Rate: | 10 pps |
| Filter Time Constant: | Normal |

Results and Discussion

The compounds analysed in this study are:

- 1. p-Toluamide
- 2. Fructose
- 3. Glucose
- 4. Sucrose
- 5. Maltose
- 6. Lactose
- 7. Maltotriose
- 8. Maltotetraose
- 9. Maltopentaose
- 10. Maltohexahose
- 11. Maltoheptaose

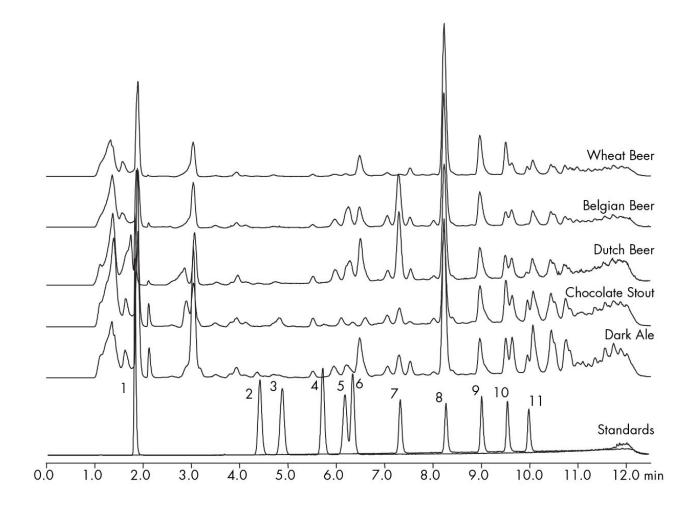

Featured Products

ACQUITY UPLC ELS Detector <https://www.waters.com/514219>

WA60125, October 2009

© 2022 Waters Corporation. All Rights Reserved.