

## Analysis of Cellulosic Hydrolysates Using ACQUITY UPLC BEH Amide Columns

---

Waters Corporation

This is an Application Brief and does not contain a detailed Experimental section.

---

### Abstract

This application brief highlights the analysis of cellulosic hydrolysates using ACQUITY UPLC BEH Amide Columns.


---

### Introduction


The compounds analysed in this study are:

1. Xylose
  2. Fructose
  3. Mannose
  4. Glucose
-


5. Sucrose
6. Cellobiose
7. Melezitose
8. Raffinose
9. Maltotriose
10. Maltotetraose
11. Maltopentaose
12. Maltohexaose
13. Maltoheptaose




Xylose

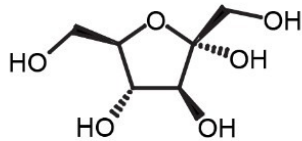


Fructose




Glucose




Mannose

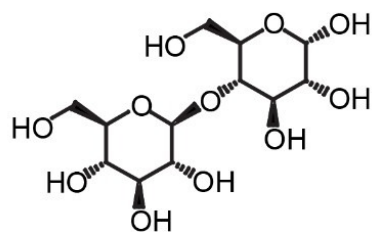


Cellobiose

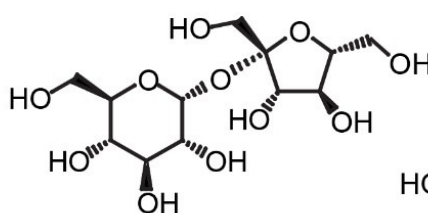


Sucrose

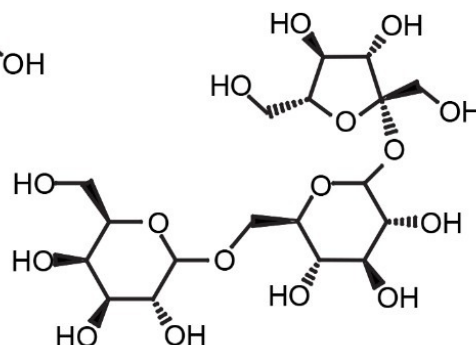

Raffinose

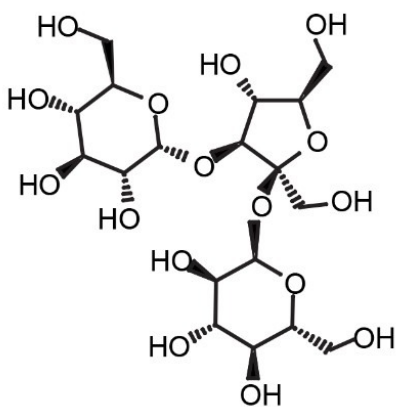

Melezitose

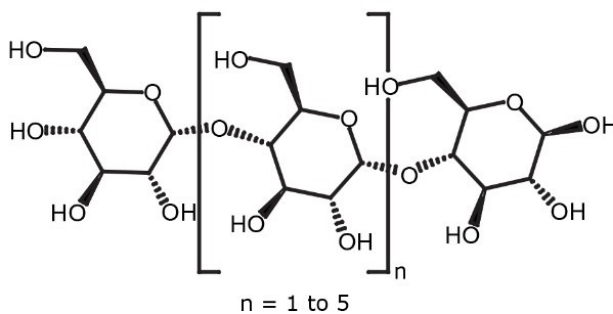

Maltooligosaccharides

---

## Experimental

### Chromatographic Conditions

Column:

ACQUITY UPLC BEH Amide 2.1 x 100 mm, 1.7

---

μm

Part Number:	186004801
Mobile Phase A:	80/20 MeCN/H <sub>2</sub> O with 0.2% triethylamine [TEA]
Mobile Phase B:	30/70 MeCN/H <sub>2</sub> O with 0.2% triethylamine [TEA]
Flow Rate:	0.12 mL/min
Gradient:	10 minute gradient, 80%-50% MeCN (w/0.2% TEA) with 30 minute re-equilibration
Injection Volume:	1.3 μL (PLNO)
Sample Concentration:	1 mg/mL each
Sample Diluent:	50/50 MeCN/H <sub>2</sub> O
Column Temperature:	35 °C
Strong Needle Wash:	20/80 MeCN/H <sub>2</sub> O (800 μL)
Weak Needle Wash:	75/25 MeCN/H <sub>2</sub> O (500 μL)
Seal Wash:	50/50 MeCN/H <sub>2</sub> O
Instrument:	Waters ACQUITY UPLC with ELSD

## Gradient


Time (min)	Profile	
	%A	%B
0.00	100.00	0.00
10.00	60.00	40.00
10.01	100.00	0.00
40.00	100.00	0.00

## ELSD Conditions

Gain:	200
Pressure:	40 psi
Drift Tube Temperature:	40 °C
Nebulizer:	Cooling
Data Rate:	10 pps
Filter Time Constant:	Normal

---

## Results and Discussion

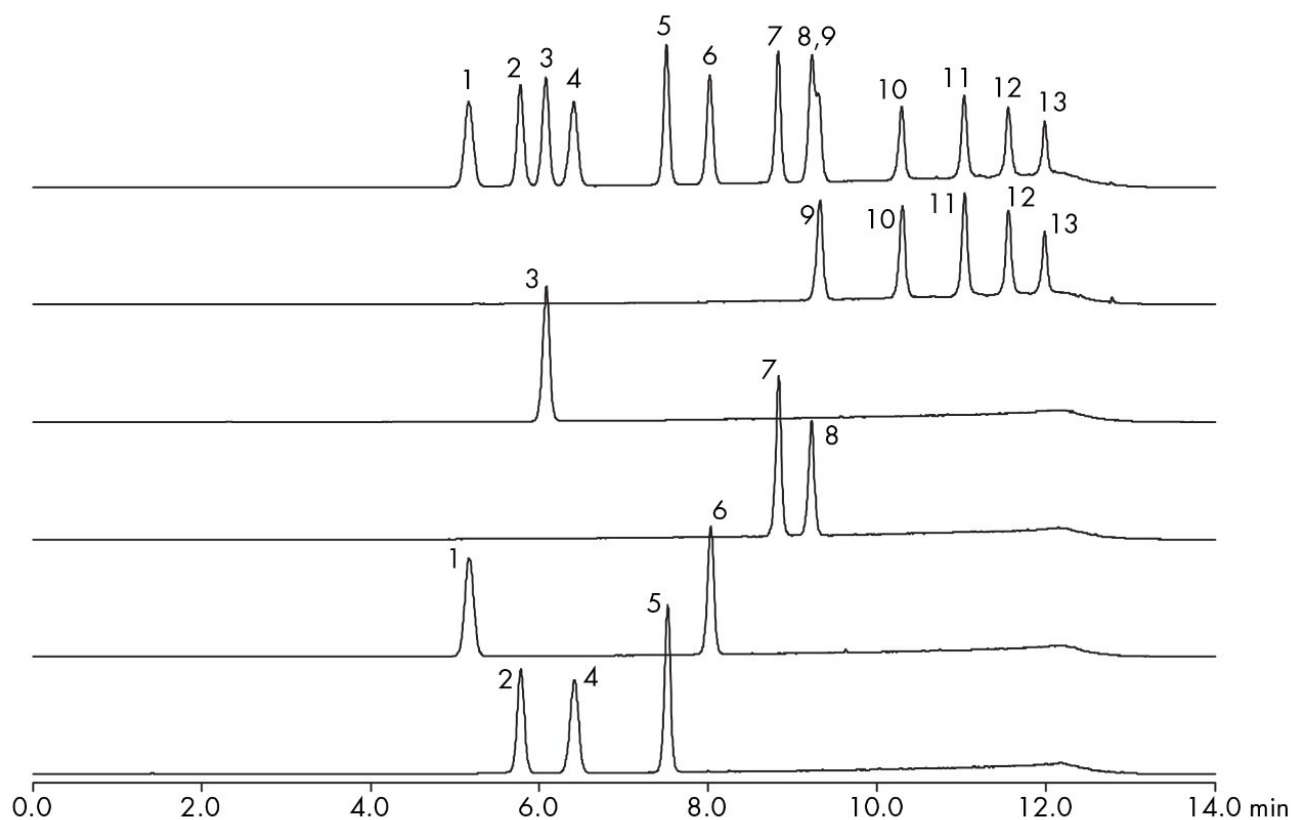

---

## Featured Products

ACQUITY UPLC ELS Detector <<https://www.waters.com/514219>>

WA60127, October 2009

© 2022 Waters Corporation. All Rights Reserved.