


Gradient Separation of Catecholamines on Atlantis HILIC Silica

Waters Corporation

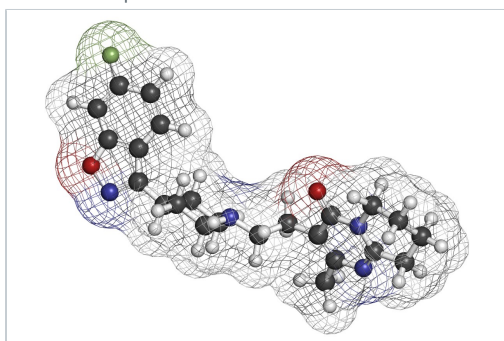

This is an Application Brief and does not contain a detailed Experimental section.

Abstract

This application brief describes the gradient separation of catecholamines on Atlantis HILIC Silica column.

Introduction

The compounds used in this study are:

1. Norepinephrine (NE)
2. Epinephrine (E)
3. 3-Hydroxytyramine (Dopamine)

Experimental


Test Conditions

Column:	Atlantis HILIC Silica, 4.6 x 50 mm, 5 μ m
Part Number:	186002028
Mobile Phase A:	H ₂ O
Mobile Phase B:	ACN
Mobile Phase C:	200 mM NH ₄ COOH, pH 3.0
Flow Rate:	2.0 mL/min
Injection Volume:	5.0 μ L
Sample Diluent:	75:25 ACN:MeOH with 0.2% FA
Sample Concentration:	42 μ g/mL Norepinephrine (NE), 17 μ g/mL Epinephrine (E), 83 μ g/mL 3-hydroxytyramine (Dopamine)
Detection:	UV @ 280 nm
Temperature:	Ambient
Instrument:	Waters Alliance System, 2695 Separations Module with 2996 PDA

Gradient:

Time(min)	Profile	
	%A	%B
0.0	0	95
5.0	25	7

Results and Discussion

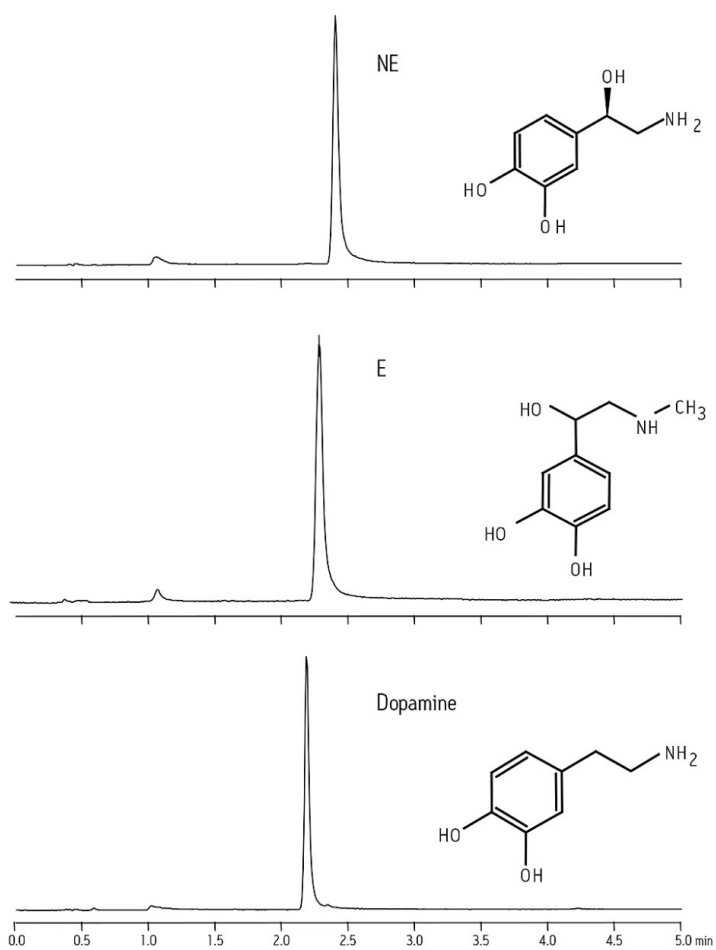

Featured Products

[Alliance HPLC System](#)

WA64073, August 2009

©2019 Waters Corporation. All Rights Reserved.