

LC-MS Gradient Separation of Buprenorphine and Buprenorphine Glucuronide on XBridge HILIC

Waters Corporation



This is an Application Brief and does not contain a detailed Experimental section.


Abstract

This application brief demonstrates the LC-MS gradient separation of buprenorphine and buprenorphine glucuronide on XBridge HILIC Columns.


Introduction

The compounds used in this study are:

1. Buprenorphine
2. Buprenorphine glucuronide

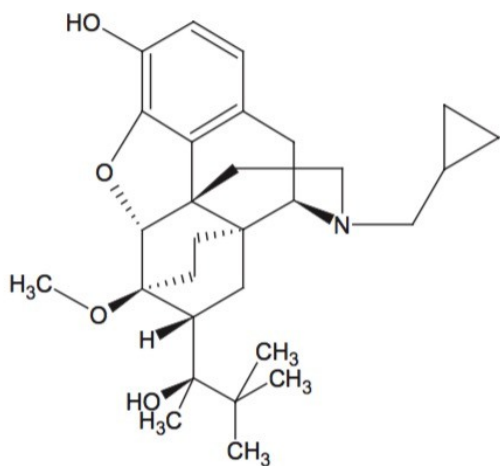

Buprenorphine

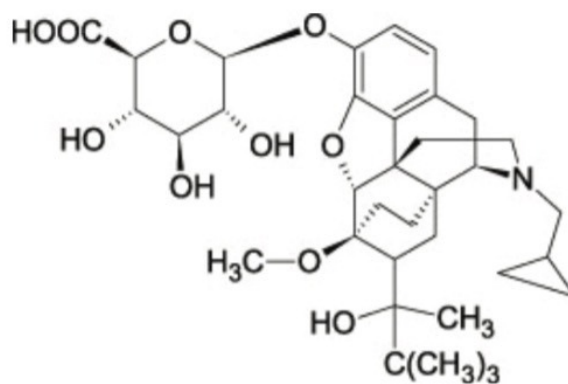

Buprenorphine glucuronide

Experimental

Method Conditions

Column:

XBridge HILIC, 3.5 μ m, 2.1 x 100 mm

Part number:

186004433


Mobile phase A:	10 mM NH ₄ COOH in H ₂ O, 0.125% HCOOH in 50:50 ACN:H ₂ O
Mobile phase B:	10 mM NH ₄ COOH in H ₂ O, 0.125% HCOOH in 90:10 ACN:H ₂ O
Flow rate:	0.3 mL/min
Injection volume:	5 µL
Sample concentration:	50 ng/mL each
Sample diluent:	75:25 ACN:MeOH with 0.2% HCOOH
Column temperature:	30 °C
Instrument:	Waters ACQUITY UPLC with TQD
MRM:	Buprenorphine 468.3 > 54.7 Buprenorphine glucuronide 644.3 > 468.3
Dwell time:	75 ms
ISD:	10 ms
ICD:	10 ms

Gradient:

Time(min)	Profile
	%A
0.00	0.1

Time(min)	Profile
1.05	0.1
4.35	99.9
5.00	99.9
5.01	0.1
6.00	0.1

Results and Discussion

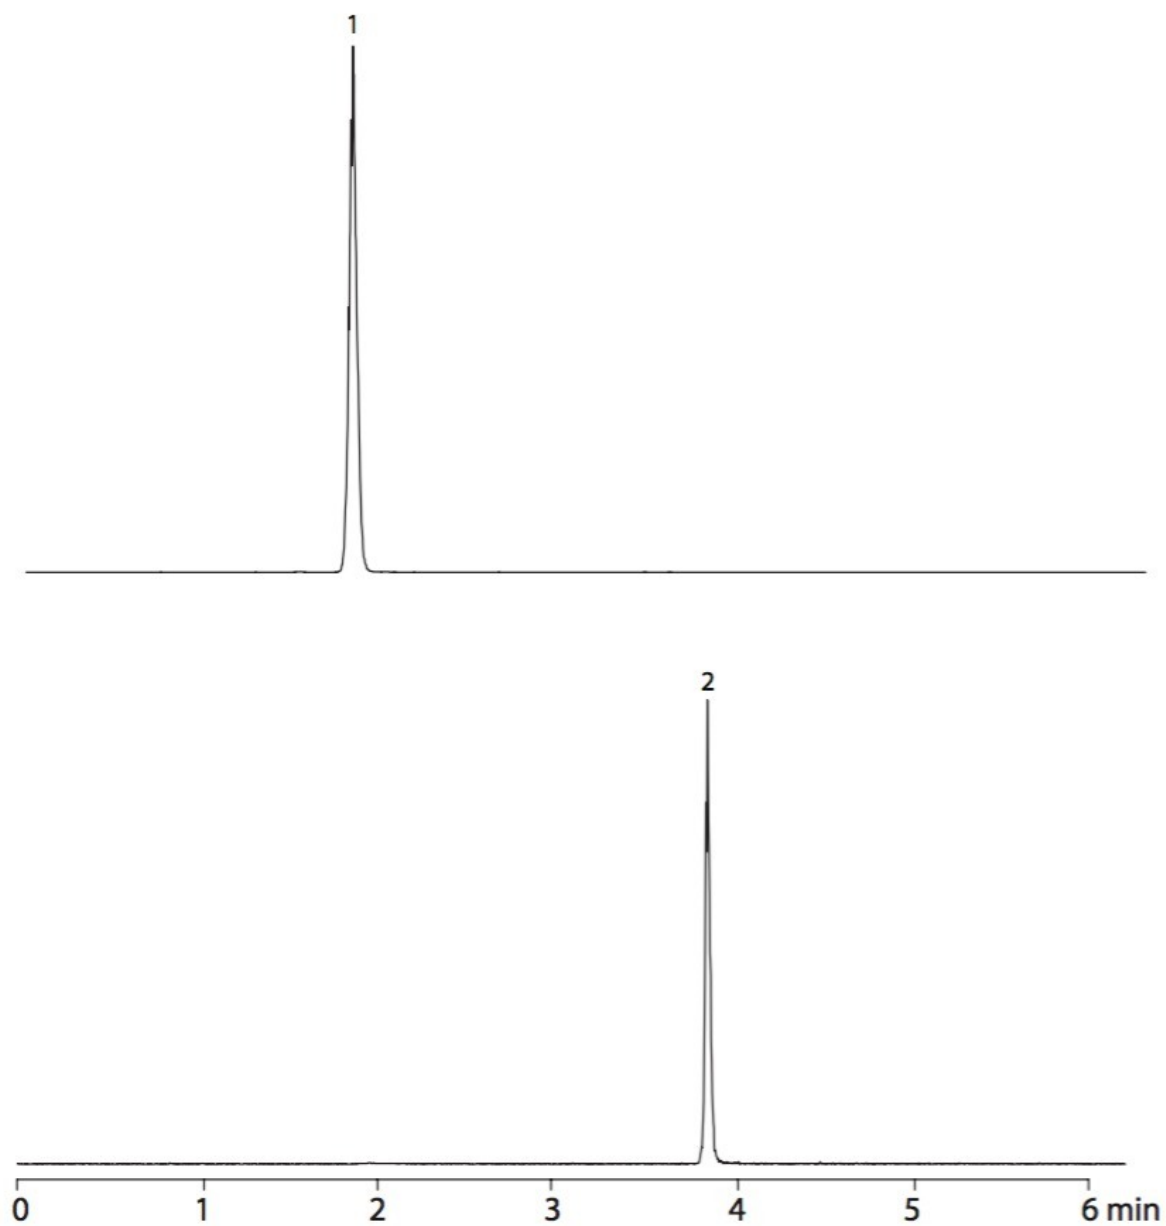

Featured Products

- [ACQUITY UPLC System <https://www.waters.com/514207>](https://www.waters.com/514207)

WA64077, August 2009



© 2021 Waters Corporation. All Rights Reserved.