

Note d'application

An Improved SPE-LC-MS/MS Platform for the Simultaneous Quantitation of Multiple Amyloid β Peptides in Cerebrospinal Fluid for Preclinical or Biomarker Discovery

Erin E. Chambers, Mary E. Lame, Diane M. Diehl

Waters Corporation, Pfizer, Neuroscience Research Unit



For research use only. Not for use in diagnostic procedures.

Abstract

In this work, the mass spectrometry platform has been updated from the Xevo TQ MS to the Xevo TQ-S mass spectrometry system. This change facilitated both a 4X reduction in required sample size and a 4-5X increase in assay sensitivity.

Benefits

- Improved sensitivity using Xevo TQ-S.
- Reduced sample size required using Xevo TQ-S.
- Fast, flexible platform for peptide quantitation.
- One LC-MS/MS method for quantitation of multiple peptides, reduced reliance on ligand-binding assays in discovery segment.
- Highly selective sample preparation using Oasis mixed-mode sorbent in μ Elution format.
- Resolution, sensitivity of ACQUITY UPLC PST columns for improved separation with shorter run times.

Introduction

A previous application note (720003682en) described in detail the development of a fast, flexible SPE-LC-MS/MS platform for the quantification of multiple amyloid beta ($\text{a}\beta$) peptides from human or monkey CSF for use in a biomarker or preclinical discovery setting. In this work, the mass spectrometry platform has been updated from the Xevo TQ MS to the Xevo TQ-S mass spectrometry system. This change facilitated both a 4X reduction in required sample size and a 4-5X increase in assay sensitivity.

Historically, quantification of $\text{a}\beta$ peptides in biological fluids has relied mainly on the use of immunoassays, such as ELISA. These assays are time consuming and expensive to develop, labor intensive, are subject to cross reactivity, and an individual assay is required for each peptide. In order to meet the throughput requirements and constant flow of demands for new peptide methods in a discovery setting, there is a need for a highly specific yet flexible methodology based on an LC-MS/MS platform. In this work, this platform is coupled with selective sample preparation for the simultaneous quantitation of multiple $\text{a}\beta$ peptides. This work focuses on methods for the 1-38, 1-40, and 1-42 $\text{a}\beta$ peptides, in support of preclinical and biomarker

discovery studies. Sequence, pI and molecular weight (MW) information for these peptides is shown in Figure 1.

Amyloid β 1-38

DAEFRHDSGYEVHHQKLVFFAEDVGSNKGAIIGLMVGG

MW 4132 pI 5.2

Amyloid β 1-40

DAEFRHDSGYEVHHQKLVFFAEDVGSNKGAIIGLMVGGVV

MW 4330 pI 5.2

Amyloid β 1-42

DAEFRHDSGYEVHHQKLVFFAEDVGSNKGAIIGLMVGGVVIA

MW 4516 pI 5.2

Figure 1. Sequence, MW, and pI information for amyloid β peptides.

The solid-phase extraction (SPE) sample preparation protocol used to enrich the amyloid beta fraction in CSF is the protocol previously described. However, the sample size required is now only 50 μ L instead of 200 μ L. The SPE method concentrates the sample to improve detection limits while eliminating matrix interferences and optimizing solubility of the a β peptides in the mass spectrometer injection solvent.

As strategies emerge for disease modification in Alzheimer's Disease (AD), the quantification of other a β species (in addition to a β 38, 40, and 42) that may be linked to AD pathology may be required. The method described herein shows promise for adaptation to quantify those peptides as well.

Experimental

UPLC conditions

Column:	ACQUITY UPLC BEH C ₁₈ 300Å, 2.1 x 150 mm, 1.7 μm, Peptide Separation Technology
Part Number:	186003687
Column temp.:	50 °C
Sample temp.:	15 °C
Injection volume:	10.0 μL
Injection mode:	Partial Loop
Flow rate:	0.2 mL/min.
Mobile phase A:	0.3% NH ₄ OH in H ₂ O
Mobile phase B:	90/10 ACN/mobile phase A
Strong needle wash:	60:40 ACN:IPA + 10% conc. NH ₄ OH (600 μL)
Weak needle wash:	90:10 0.3% NH ₄ OH in H ₂ O:ACN (400 μL)

Gradient

Time (min)	%A	%B	Curve
0.0	90	10	6
1.0	90	10	6
6.5	55	45	6
6.7	55	45	6

Time (min)	%A	%B	Curve
---------------	----	----	-------

70	90	10	6
----	----	----	---

Waters Xevo TQ-S MS conditions, electrospray positive

Capillary Voltage:	2.5 V
Desolvation Temp:	450 °C
Cone Gas Flow:	Not used
Desolvation Gas Flow:	800 L/Hr
Collision Cell Pressure:	2.6 x 10 ⁽⁻³⁾ mbar
MRM transition monitored, ESI+:	See Table 1

Peptide Name	Precursor Ion 4+	Product Ion 4+	Product Ion i.d.	Cone Voltage (V)	Collision Energy (eV)
Amyloid β 1-38	1033.5	1000.3	b 36	33	23
Amyloid β 1-38 N15 IS	1046	1012.5		30	22
Amyloid β 1-40	1083	1053.6	b 39	33	25
Amyloid β 1-40 N15 IS	1096	1066.5		35	22
Amyloid β 1-42	1129	1078.5	b 40	28	30
Amyloid β 1-42 N15 IS	1142.5	1091.5		35	28

Table 1. MRM transitions and MS conditions for the amyloid β peptides and their N15 labeled internal standards.

SPE conditions

Sample pre-treatment

50 µL human CSF or spiked artificial CSF + 5% rat plasma was diluted 1:1 with 5 M guanidine HCL and shaken at room temperature for 45 minutes. This was then diluted further with 50 µL 4% H₃PO₄ in H₂O and

mixed.

Note: For spiked samples, samples were allowed to equilibrate at room temperature for 30 min after spiking and prior to dilution with guanidine HCl.

Sample extraction with Oasis MCX

Samples were extracted according to the protocol in Figure 2 below. All solutions are made up by volume. All steps applied to wells of μ Elution plate containing samples

Oasis MCX μ Elution protocol (Part Number: 186001830BA)

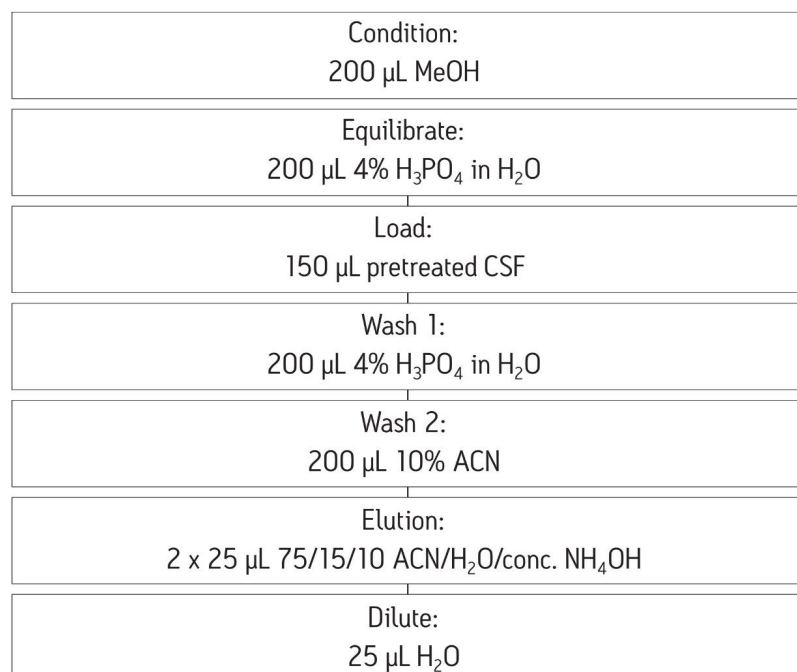


Figure 2. Oasis μ Elution MCX extraction protocol

Results and Discussion

Mass Spectrometry

MS was performed in positive ion mode since CID of the 4+ precursor ion yielded several distinct product

ions corresponding to specific b sequence ions (representative spectrum shown in Figure 3.)

The sensitivity increase provided by the Xevo TQ-S facilitated the use of 4X less sample whilst also improving detection limits by approximately 4-5X compared to the previous assay on the Xevo TQ. The lowest QC sample tested was 5X lower in concentration than the low QC when the standard Xevo TQ MS system was used. Earlier work by Rainville and Booth (application note 720003415en) describes the system improvement in more depth and demonstrates a similar sensitivity increase for the therapeutic peptide desmopressin.

Mass range of the instrument was also an important factor in obtaining specificity. The Xevo TQ-S MS has a mass range of 2048 on both quads, easily allowing us to choose a more specific 4+ rather than 5+ precursor and fragment pair.

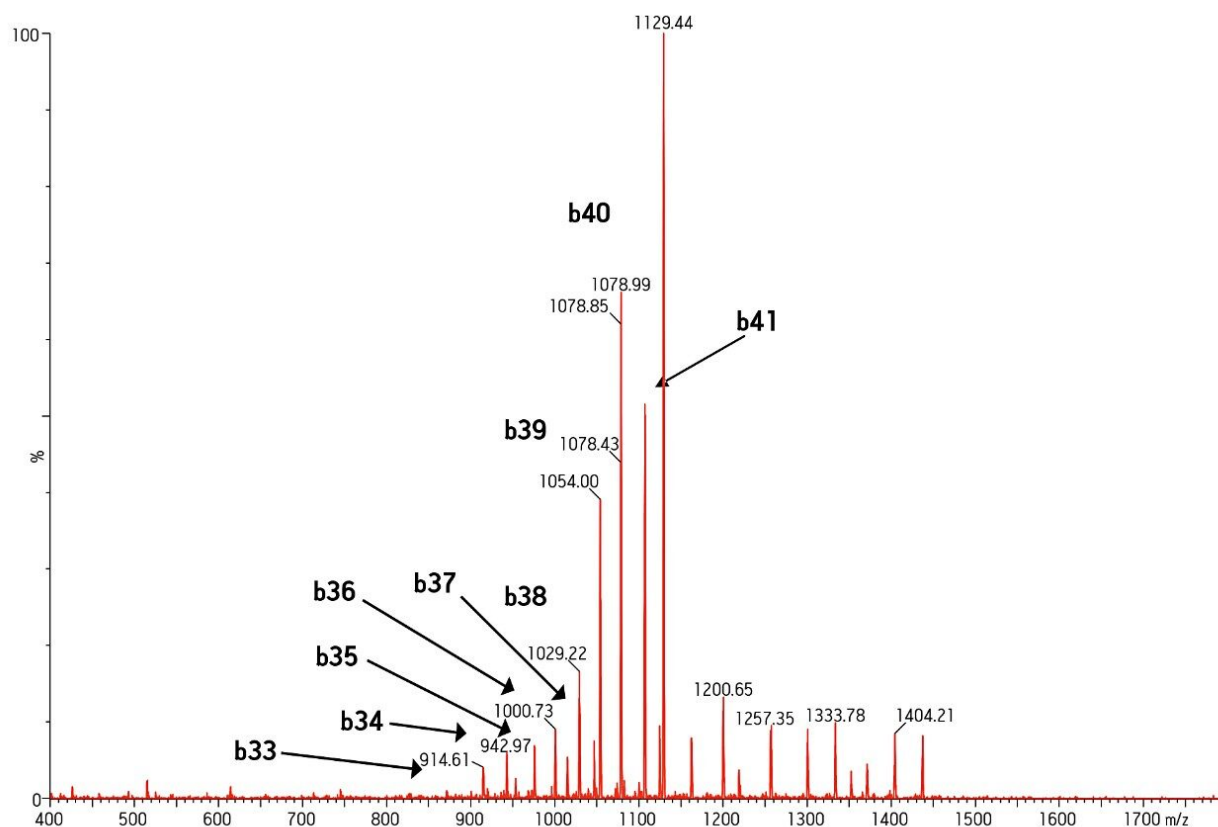


Figure 3. Representative ESI+ MS/MS spectrum for amyloid β 1-42 with fragment sequence ions labeled.

UPLC separation

Separation of the three amyloid β peptides is shown in Figure 4. While the exact amount of NH_4OH in the mobile phase was critical for negative ion sensitivity, the signal in ESI positive proved to be more robust to

subtle changes in mobile phase composition, providing a minimum of >24 hour LC/autosampler stability. In contrast, 50% or more of the ESI negative signal was lost after 10-12 hours due to the natural change in NH_4OH concentration (volatility) in the mobile phase. This further reinforced the robustness of an ESI positive MS method.

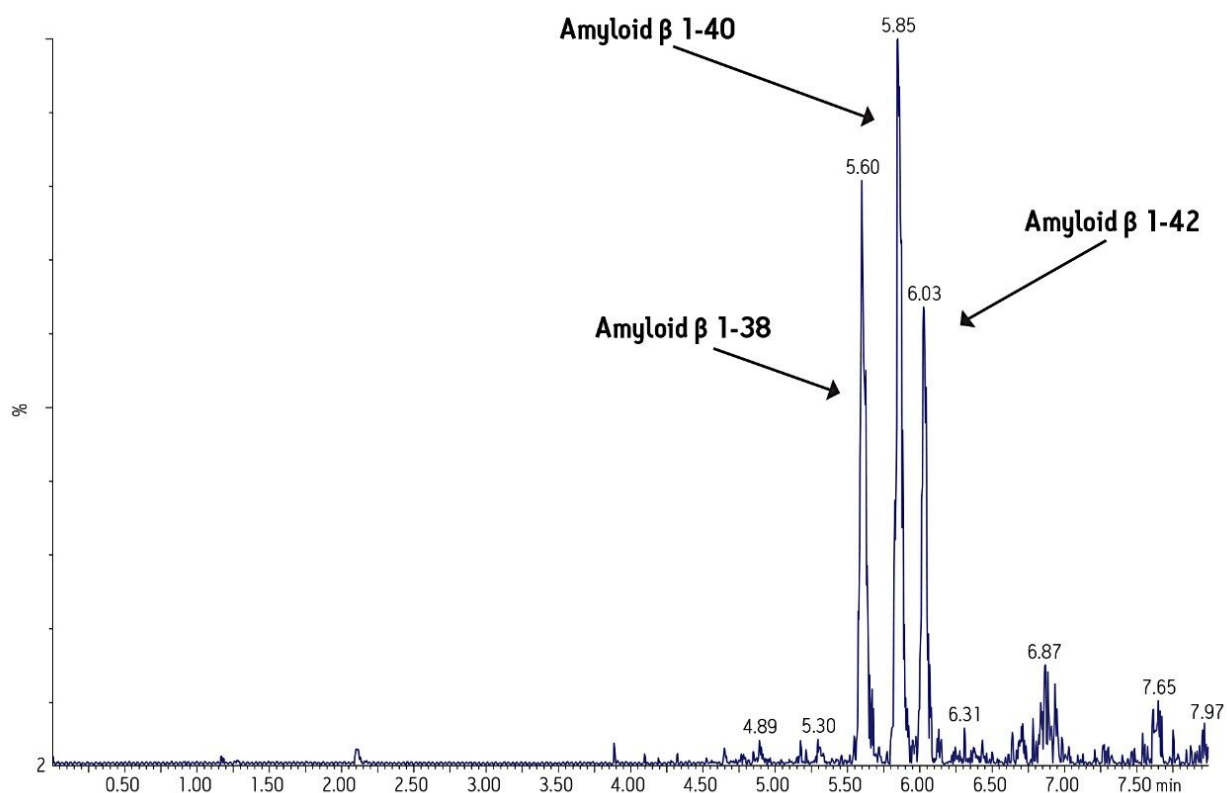


Figure 4. Representative UPLC-MS/MS analysis of amyloid β 1-38, 1-40, and 1-42 peptides extracted from artificial CSF + 5% rat plasma.

Sample preparation: SPE

SPE was performed using Oasis MCX, a mixed-mode sorbent, to enhance selectivity of the extraction. The sorbent relies on both reversed-phase and ion-exchange retention mechanisms to selectively separate the $\text{a}\beta$ fraction from other high abundance polypeptides in complex CSF samples. The Oasis μ Elution plate (96-well format) provided sample concentration, eliminating the need for evaporation and reconstitution. This has the benefit of saving time and eliminating peptide losses due to adsorption to the walls of the collection plate during dry down.

During initial method development, a high degree of non-specific binding (NSB) was observed when artificial

CSF was extracted. Thus, 5% rat plasma (having a different amyloid β sequence) was added to bind to surfaces, eliminating NSB.

The SPE method was one of the more critical aspects of the overall methodology. Very selective isolation of the amyloid fraction coupled with the resolution of analytical-scale flow UPLC, facilitates analysis of pre-clinical samples without the need for antibodies or time-consuming immuno-precipitation associated with ELISA methods. The increased sensitivity of the Xevo TQ-S enabled the sample volume to be reduced from 200 μ L to 50 μ L of CSF, making this method amenable to use in pre-clinical species.

Peptide Name	200 μ L Sample Xevo TQ	50 μ L Sample Xevo TQ-S
Standard Curve Range	0.1-10 ng/mL	0.025 or 0.05-10 ng/mL
QC Range	0.2-6 ng/mL	0.04-6 ng/mL

Table 2. Comparison of standard curve and QC range using Xevo TQ and TQ-S MS.

Name	Type	Std. Conc.	RT	Area	IS Area	Response	Conc.	%Dev
Blank artificial CSF			5.73	19.7	7.0			
50 pg/mL artificial CSF	Standard	0.05	5.71	230.4	3620.5	0.064	0.057	14
100 pg/mL artificial CSF	Standard	0.1	5.71	390.8	3585.1	0.109	0.108	8.1
250 pg/mL artificial CSF	Standard	0.25	5.71	778.3	3737.3	0.208	0.220	-12
350 pg/mL artificial CSF	Standard	0.35	5.71	1267.3	3693.8	0.343	0.372	6.2
500 pg/mL artificial CSF	Standard	0.5	5.71	1494.7	3566.8	0.419	0.457	-8.5
750 pg/mL artificial CSF	Standard	0.75	5.71	2733.5	4152.0	0.658	0.727	-3.1
1 ng/mL artificial CSF	Standard	1	5.71	3166.8	3792.5	0.835	0.926	-7.4
5 ng/mL artificial CSF	Standard	5	5.72	14773.9	3148.3	4.693	5.270	5.4
7.5 ng/mL artificial CSF	Standard	7.5	5.72	24576.9	3877.0	6.339	7.125	-5
10 ng/mL artificial CSF	Standard	10	5.72	33343.3	3662.5	9.104	10.238	2.4

Compound name: Amyloid BEta 1-42
 Correlation coefficient: $r = 0.998799$, $r^2 = 0.997600$
 Calibration curve: $0.887923 \cdot x + 0.0130161$
 Response type: Internal Std. (Ref 2), Area*(IS Conc. /IS Area)
 Curve type: Linear, Origin: Exclude, Weighting: 1/x, Axis trans.: None

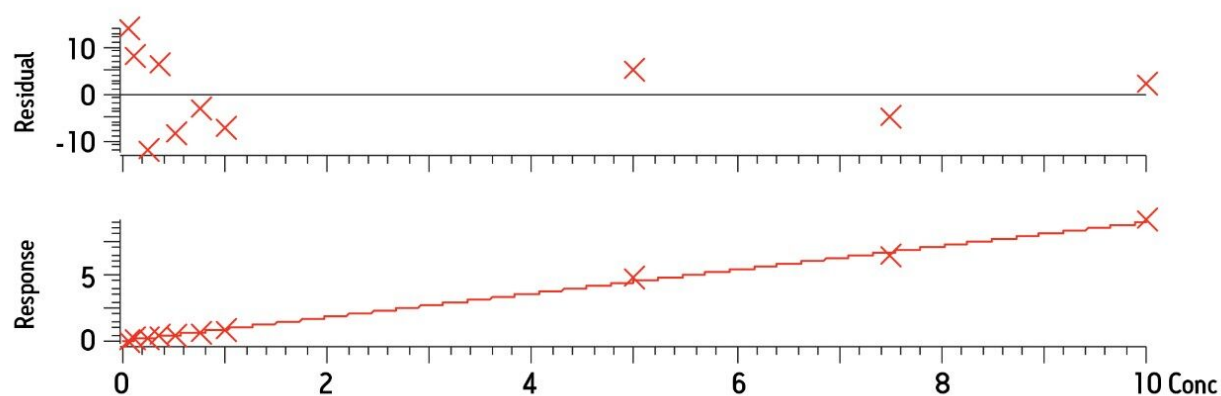


Figure 5. Representative standard curve and statistics from 0.05-10 ng/mL for amyloid β 1-42 extracted from artificial CSF + 5% rat plasma.

	Average Basal Level	% RSD of Basal Level	IS % RSD
Amyloid β 1-38 Human CSF 1	1.396	5.3	6.4
Amyloid β 1-38 Human CSF 2	0.702	1.7	
Amyloid β 1-40 Human CSF 1	5.429	3.3	4.7
Amyloid β 1-40 Human CSF 2	2.611	2.7	
Amyloid β 1-42 Human CSF 1	0.458	5.2	6.6
Amyloid β 1-42 Human CSF 2	0.226	1.9	

Table 3. Baseline levels of amyloid β peptides in 2 sources of pooled human CSF.

	QC 0.04 ng/mL	QC 0.075 ng/mL	QC 0.15 ng/mL	QC 0.2 ng/mL	QC 0.8 ng/mL	QC 2 ng/mL	QC 6 ng/mL
Amyloid β 1-38 Human CSF 1 and 2	2.3	5.8	-3.2	7.3	14.8	5.1	13.1
Amyloid β 1-40 Human CSF 1 and 2	-0.8	-3.2	-1.9	2.5	-2.6	-4.2	-3.8
Amyloid β 1-42 Human CSF 1 and 2	1.3	13.4	-3.6	5.6	2.0	-0.6	-0.2

Table 4. Average deviation values for all overspike QC samples.

Conclusion

- The increased sensitivity of the Xevo TQ-S triple quadrupole mass spectrometer facilitated the use of 4X less sample and a 4-5X improvement in quantification limits.
- An SPE-UPLC-MS/MS bioanalytical method was developed and validated for the simultaneous quantitation of multiple amyloid β peptides in human and monkey CSF.
- The combination of a highly selective extraction method based on mixed-mode SPE in μ Elution format and the resolution of UPLC chromatography was critical to achieving the accurate, precise and reliable quantitation of 3 major amyloid β peptides in human and monkey CSF.
- The use of positive ion MS/MS and b ion sequence fragments provided the MS specificity required for this application.
- 96 samples can be extracted and ready for injection in <30 minutes, providing the sample prep throughput required for pre-clinical and clinical studies.
- The method described herein eliminates time-consuming immunoassays or immunoprecipitation steps for pre-clinical work.
- This approach also allows one assay for the simultaneous measurement of several different amyloid β peptides from a single sample. This single assay provides a high degree of selectivity and specificity in a high-throughput format while still achieving the high sensitivity required for low level endogenous amyloid β peptides.
- The use of a single UPLC-MS/MS assay represents a significant advantage over an ELISA assay, which would require multiple assays with multiple antibodies to quantify each of the relevant peptides.

References

1. T.A. Lanz, J.B. Schachter, *Journal of Neuroscience Methods* 169 (2008) 16-22.
2. T. Oe *et al*, *Rapid Communications in Mass Spectrometry* 20 (2006) 3723-3735.
3. JR Slemmon *et al*, *Journal of Chromatography B* 846 (2007) 24-31.
4. NT Ditto *et al*, *Journal of Neuroscience Methods* 182 (2009) 260-265.
5. T.A. Lanz, J.B. Schachter, *Journal of Neuroscience Methods* 157 (2006) 71-81.
6. MJ Ford *et al*, *Journal of Neuroscience Methods* 168 (2008) 465-474.
7. E. Portelius *et al*, *Journal of Proteome Research*, 6 (2007) 4433-4439.

Featured Products

[ACQUITY UPLC System <https://www.waters.com/514207>](https://www.waters.com/514207)

[Xevo TQ-S <https://www.waters.com/10160596>](https://www.waters.com/10160596)

720003860, February 2011