

The Determination of Fruit Juice Authenticity Using High Resolution Chromatography, UV, Time-of-Flight MS, and Multivariate Analysis

Marian Twohig, Antonietta Gledhill, Jennifer A. Burgess

Waters Corporation

Abstract

In this application note, we illustrate how the combination of Waters' UltraPerformance Liquid Chromatography (UPLC) system for high-resolution separations, ACQUITY UPLC Photodiode Array (PDA), eλ Detector, and accurate mass Xevo G2 QToF MS, with the appropriate chemometric software tools, allow easy and rapid differentiation between authentic and adulterated pomegranate juice samples.

Benefits

- Provides juice chemists with a powerful system solution to comprehensively research existing and new juice product prototypes in a fast-paced marketplace.
 - Allows easy and rapid differentiation between authentic and adulterated pomegranate juice samples.
 - Multivariate statistical analysis (MVA) enables visualization and interpretation of complex MS data sets.
 - QToF MS provides simultaneous accurate mass information, for both the precursor and fragment ions in a single injection.
-

Introduction

The verification of food sources and authenticity is an activity that has increased in importance over the last decade. The adulteration of food and beverages has emerged as a growing problem that can pose potential threats to the health of consumers and to the integrity of the industry¹. Economic adulteration and other types of counterfeiting in the food and consumer products industries are estimated to cost between \$10 and \$15 billion USD per year.²

There are different types of adulteration that can occur, as illustrated in Figure 1. While some types can be harmful to health³ (melamine is a good example of this); others can be very misleading to the consumer – especially if they believe the product is beneficial for certain health conditions. To date, reported cases of fruit juice adulteration primarily include the addition of highfructose corn syrup (HFCS) or blending with other fruit juices.

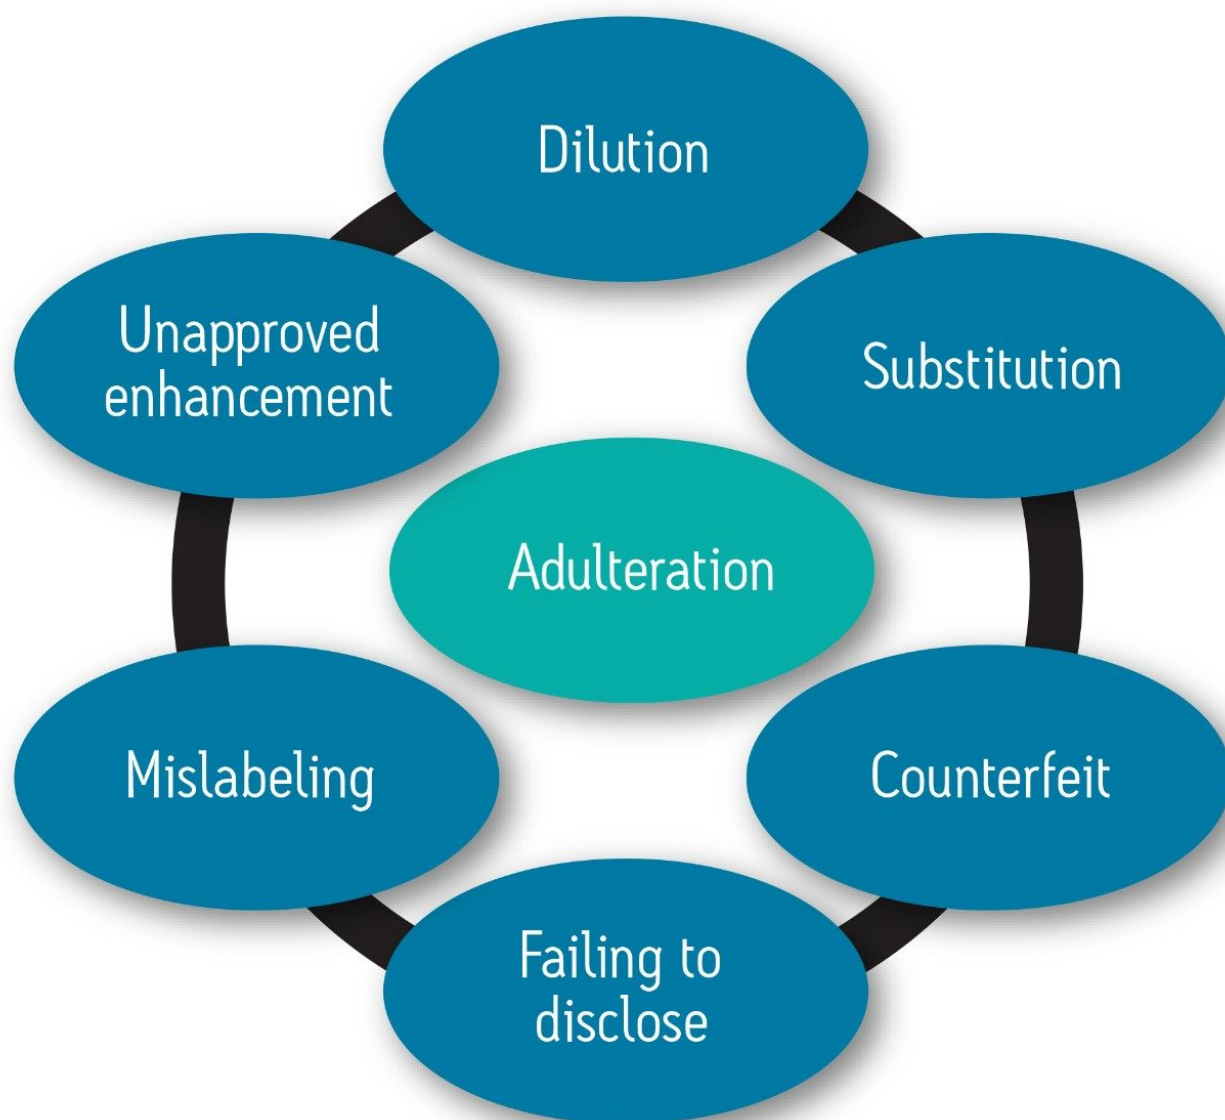


Figure 1. Flow diagram showing various ways of food adulteration

Consumer demand for some fruit juices, such as pomegranate juice, has increased significantly in recent years as clinical studies indicate that there may be positive health benefits associated with the consumption of the fruit and the juice form. These health benefits include the prevention against cancer and cardiovascular disease.⁴⁻⁷ For this reason, pomegranate juice has gained a reputation for being a super fruit – with demand often exceeding supply. As a result, the practice of adulterating pomegranate juice with lower quality juices has

become prevalent.⁸

One of the issues the fruit juice industry faces is in the research and development of new and exotic juice varieties. While many of the common fruit juices that have been in the marketplace for many years are analytically well documented and studied, this is not always the case for the newer juices that are now available. For these types of products, there is a need for sophisticated testing methods to help authenticate ingredients and finished products.

In this application note, we illustrate how the combination of Waters Ultra Performance Liquid Chromatography (UPLC) System for high-resolution separations, ACQUITY UPLC Photodiode Array (PDA), eλ Detector, and accurate mass Xevo G2 QTof MS, with the appropriate chemometric software tools, allow easy and rapid differentiation between authentic and adulterated pomegranate juice samples.

Experimental

Sample description

A description of the pomegranate samples is provided in Table 1.

Name	Sample description	Sample type
S1	Study sample – Adulterated	Juice
S2	Study sample – Authentic	Juice
S3	Study sample – Adulterated	Juice
S4	Study sample – Authentic	Juice
S5	Study sample – Unknown history	Juice
S6	Purchased-Blend	Juice
Whole fruit	Three whole pomegranates	Skin, arils, pulp

Table 1. Description of the pomegranate samples used for the analysis.

Juice samples:

Three pomegranate juice concentrate samples were obtained from a collaborator: one authentic (S2) and two adulterated (S1 and S3). Commercially available pomegranate juice samples were also included in the experiment (S4-S6). Consultation with industry experts confirm that the sample labeled S4 is believed to be 100% authentic pomegranate juice.

The juice concentrates were made up to single dose (160 Brix). One degree Brix is one-gram of fruit soluble solids in 100 grams of solution, and thus represented the strength of the solution as a percentage by weight (%)

w/w). All samples were centrifuged, filtered, and diluted before analysis.

Pomegranate fruit:

Whole fruit pomegranates were dissected into three components: arils, pulp, and skin. Each component was homogenized, centrifuged, and filtered before analysis.

UPLC conditions

LC system:	ACQUITY UPLC
Column:	ACQUITY HSS T3, 2.1 x 100 mm, 1.8 μ m
Column temp:	45 °C
Flow rate:	0.4 mL/ min
Mobile phase A:	10 mM Ammonium acetate in water
Mobile phase B:	Acetonitrile

UPLC Gradient

Time (min)	% Age A	% Age B
0.00	99	1
0.75	99	1
2.00	95	5
3.00	95	5
6.50	45	55
8.50	10	90
9.00	10	90
9.10	99	1

UV conditions

Detector: ACQUITY UPLC PDA Detector

Range: 210 to 500 nm

Sampling rate: 20 pts/s

Filter constant: 0.1

MS conditions

MS System: Xevo G2 QTof

Ionization mode: ESI negative (ESI-)

Analyzer mode: Resolution

Capillary voltage: 2.0 kV

Cone voltage: 25 V

Desolvation temp.: 450 °C

Desolvation gas: 900 L/Hr

Source temp.: 130 °C

MS^E Low energy CE: 4 eV

MS^E High energy CE: 15 to 45 eV

Acquisition range: 50 to 1200 *m/z*

Scan time: 0.1 sec

Lock mass reference: Leucine enkephalin

Data analysis

Data analysis and trending were performed using MarkerLynx XS Application Manager, which enables the user

to perform multivariate analysis (MVA). Spectral interpretation used EleComp, ChemSpider, and MassFragment Software to help identify the structures of unknown marker compounds.

Results and Discussion

All samples were analyzed using UPLC, PDA, and QToF MS. Typical chromatograms are shown in Figure 2. Replicate injections of the pomegranate samples (in random sequence order) were used to ensure that any experimental trends observed were directly associated to the sample.

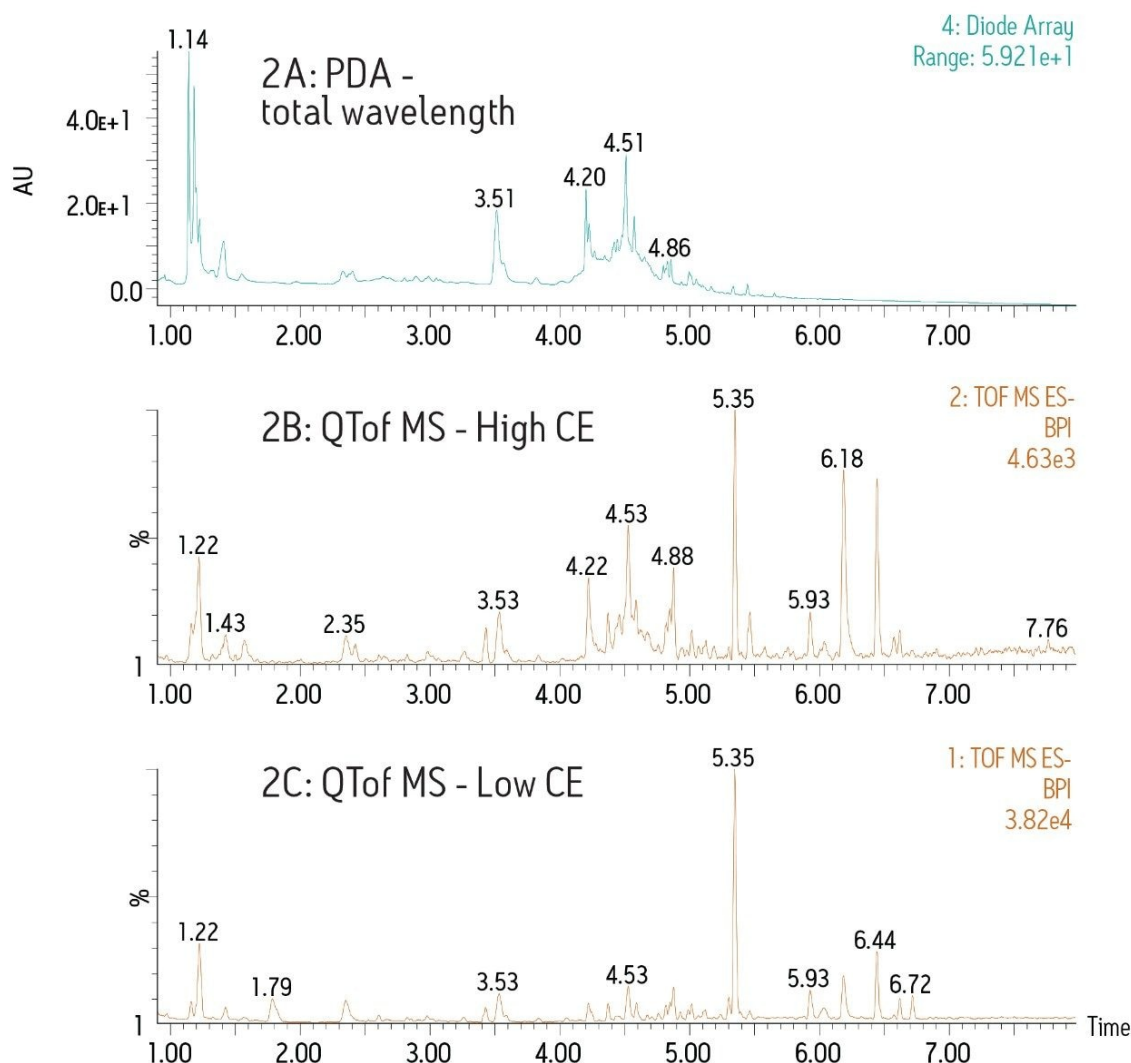


Figure 2. UPLC-PDA/QToF-MS chromatograms from the analysis of a pomegranate juice sample.

Data from the Xevo G2 QToF MS provided simultaneous accurate mass information, for both the precursor and fragment ions in a single injection. Two separate functions from the MS were produced. It is this spectral information that enables potential structural identification of unknown marker compounds.

The low collision energy chromatogram shown in Figure 2C provided the exact mass precursor ion information, and the high collision energy, shown in Figure 2B gave the exact mass fragment ion data. The ability to cycle between low and high collision energy to obtain both precursor and fragment ion information within one analysis

is a unique feature of the Waters QToF MS systems – this capability is called MS^E.

The MS data were interpreted using a Multivariate Approach (MVA) using the MarkerLynx XS Application Manager. The software performs automatic data integration and alignment to generate Exact Mass Retention Time (EMRT) pairs.

These EMRT pairs can then be used for multivariate statistical analysis to enable visualization and interpretation of complex MS data sets.⁹ The complete software workflow used in these experiments is described in Figure 3.



UPLC and Xevo G2 QTof:
High resolution chromatographic separation
High sensitivity and accurate mass



MarkerLynx XS:
Process and extract peaks
Use chemometrics to ID marker compounds



MS^E and ChemSpider:
Structural elucidation of identified marker compounds



MassFragment:
Evaluate proposed structure and searched compound



MS/MS measurement:
Acquire standards and compare standard results with samples

Figure 3. Pomegranate juice profiling workflow.

Figure 4 shows the six juice samples interpreted using Principal Component Analysis (PCA). The scores plot helps to visualize the patterns, trends, and similarities between samples. Each point in the scores plot represents a single injection. The repeat injections of each sample set are very close, indicating good repeatability.

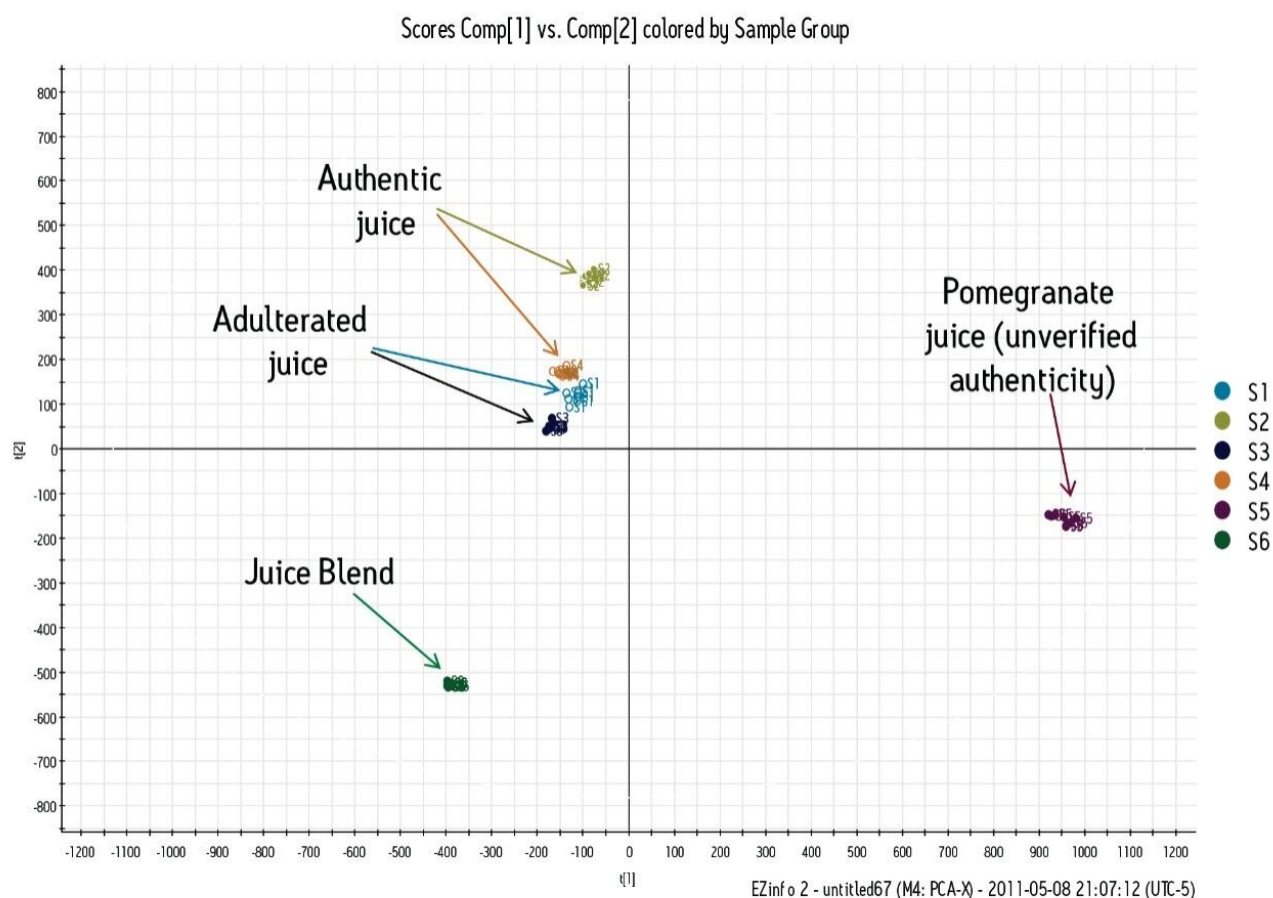


Figure 4. The scores plot obtained on analysis of six of the pomegranate juice samples using UPLC-QToF-MA MS data. (Each color represents a sample, and each sample was injected six times).

To explain the relationship between the potential markers (EMRTs) and relate these to the score plots, one approach (when looking at multiple samples) is to use a loadings plot, as shown in Figure 5. It is then possible to highlight EMRT's in the loadings plot and track their abundance using a variable trend plot.

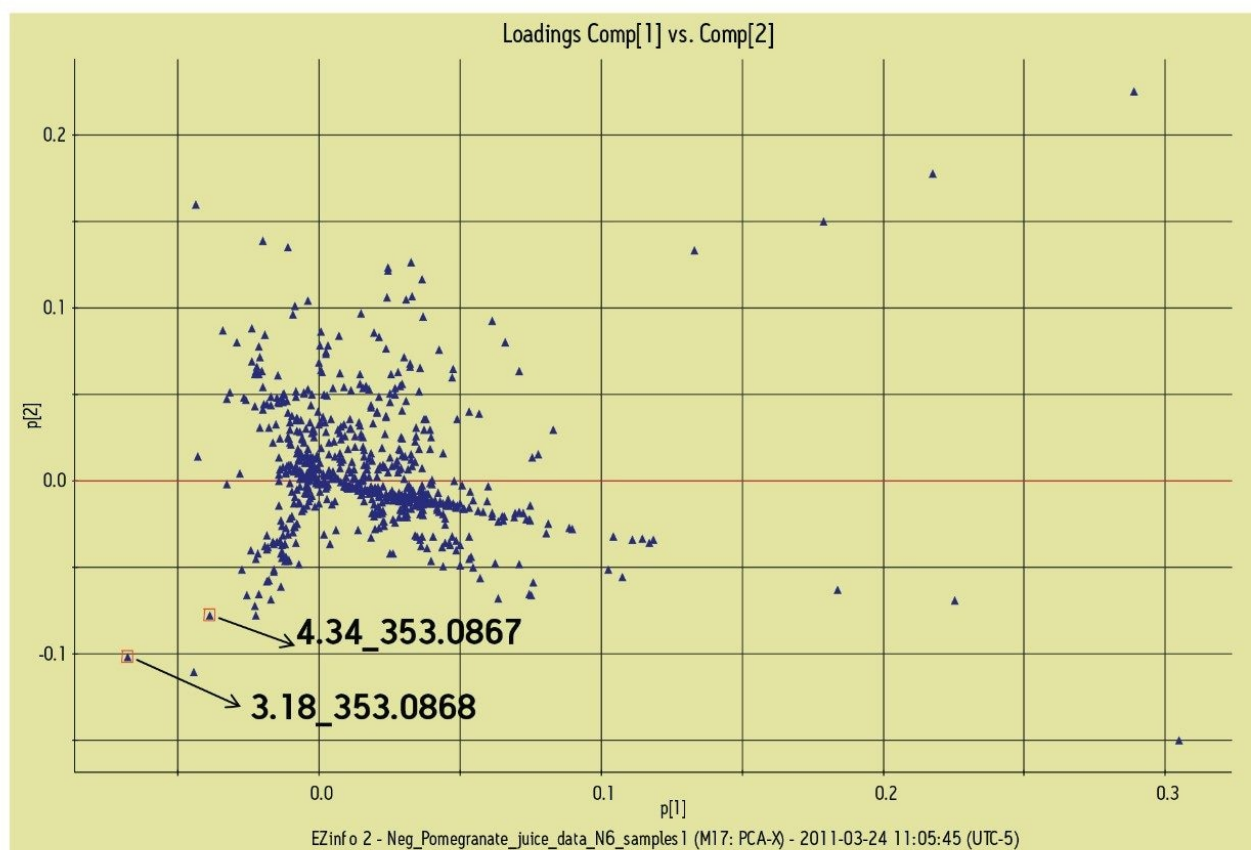


Figure 5. Loadings plot obtained from the analysis of the for the six pomegranate juice samples (UPLC-QToF-MS data); Each symbol in the loadings plot represents a single EMRT pair: where 4.34 is retention time and 353.0867 is the exact mass (m/z).

Using both the loadings plot and the variable trend plot, it can be seen that two EMRTs, with m/z 353.0868 at retention times (Rts) 3.18 and 4.34 min are absent in the known authentic samples (S2 and S4), and S5 (a sample of unverified authenticity), as shown in Figure 6.

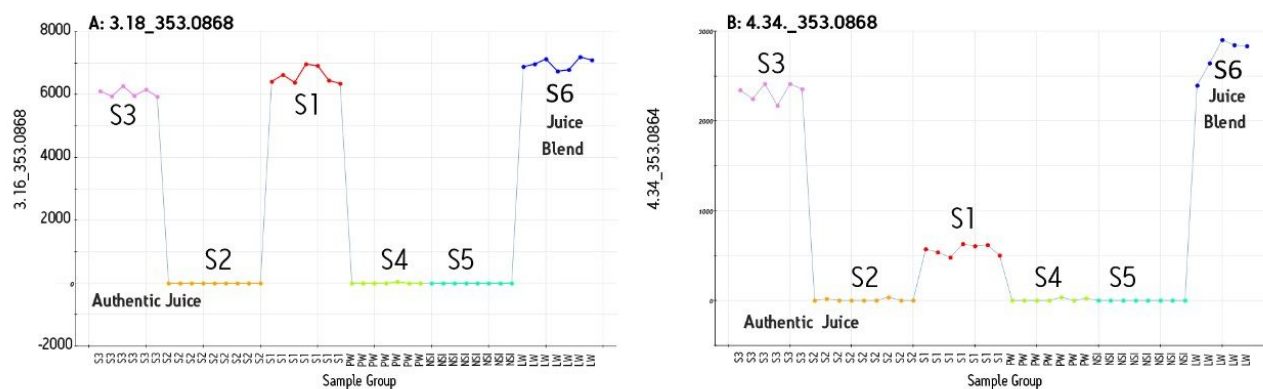


Figure 6. Variable trend plots for two possible markers (with m/z 353.0868) at R_t 3.18 min (A) and R_t 4.34 min (B).

Identification of chlorogenic acid

The presence of these two EMRT pairs at R_t s 3.18 and 4.34 min was clearly evident in the deliberately adulterated juice samples and the juice blend. The elemental composition for both components was determined to be $C_{16}H_{17}O_9$. Searching the formula in ChemSpider (an online database) proposed chlorogenic acid as the top hit. Following the workflow described in Figure 3, MassFragment Software was used to determine whether the fragments seen in the MS^E data matched possible fragments for this compound. The results indicated that chlorogenic acid matched well.

To confirm the identity of this potential marker, a standard of chlorogenic acid was analyzed and this standard eluted at a retention time of 3.18 min, shown in Figure 7A, which was the same retention time as one of the peaks in the samples, shown in Figure 7B.

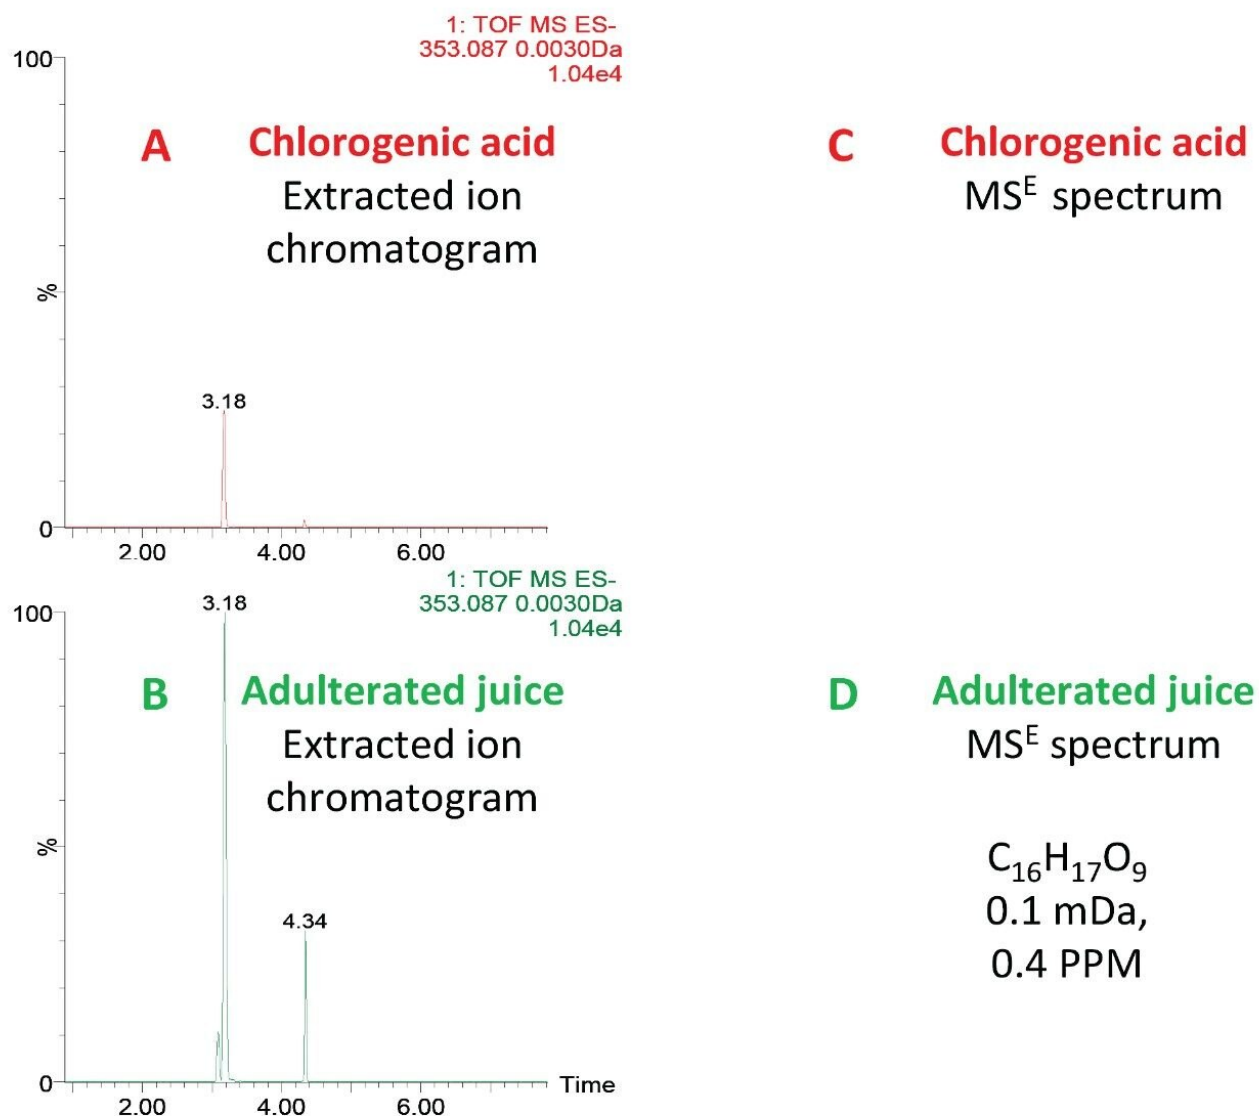


Figure 7. Extracted ion chromatograms (m/z 353.0873) for chlorogenic acid $[M-H]^-$ in a standard (7A) and an adulterated pomegranate juice sample, S3 (7B). High CE MS^E spectra for standard (7C), and sample (7D) are also shown.

The UV spectra of the standard chlorogenic acid and the peak in the sample were compared. The UV spectra taken across the entire peak width was inconclusive due to co-elution of other compounds in the samples. The MS data was then investigated and the low energy precursor ions and high energy fragment exact mass ions

provided excellent confirmation that the component at Rt 3.18 min was chlorogenic acid, as shown in Figures 7C and 7D.

The MS^E data for the component at Rt 4.34 min revealed that while it shared some common fragments with chlorogenic acid, it also showed additional fragments. This suggests that this component may be a possible isomer of chlorogenic acid (data not shown).

A closer look at the adulterated samples (S3 and S1) and the juice blend (S6), show that they all contain chlorogenic acid (*m/z* 353.0873 at 3.18 min) and possible isomers at 4.34 min and 3.09 min.

Analysis of other fruit juices showed that chlorogenic acid was also identified in authentic peach, cranberry, and blueberry juice samples (data not shown).

Eleven additional pomegranate juice samples, all claiming to be made from 100% authentic pomegranate juice or juice concentrate were purchased and analyzed. The LC-MS^E data revealed the presence of chlorogenic acid in five of the samples tested. Two of those five samples were made from imported juice and juice concentrate from Turkey. Poyrazoglu et.al have reported the presence of chlorogenic acid in 13 different pomegranate varieties from four growing regions in Turkey using LC/UV.¹⁰

Whole fruit experiments

Experiments were then performed on whole fruit samples to determine whether chlorogenic acid is present in pomegranate. Three whole fruit pomegranates (all believed to be grown in North America) were purchased and dissected into three components: arils, pulp, and skin. The pomegranate segments were extracted and analyzed.

Using the same analytical conditions as for the juice, chlorogenic acid could not be found in any part of the pomegranates, as shown in the extracted ion chromatograms in Figure 8.

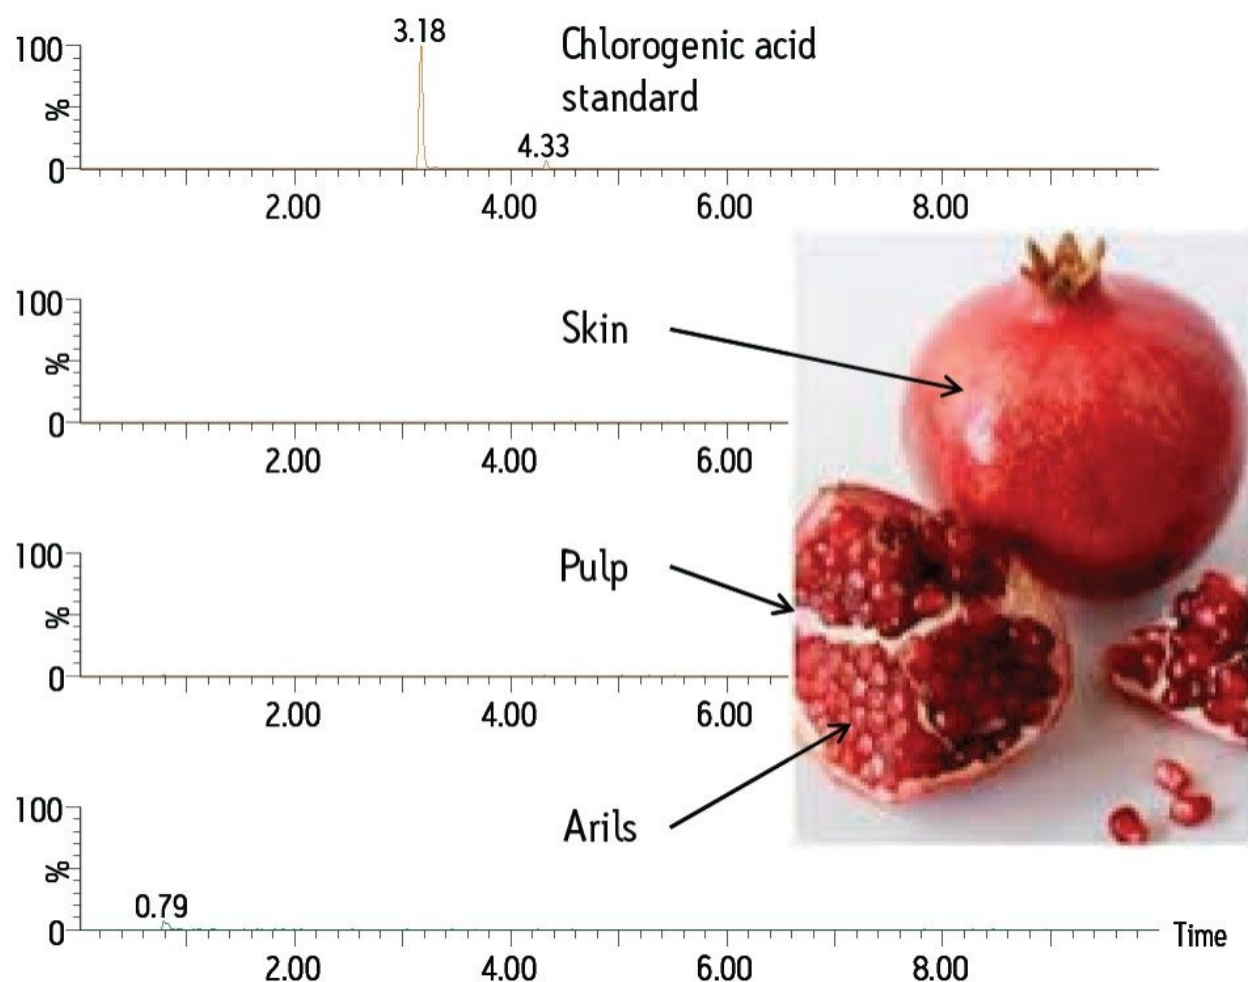


Figure 8. Extracted ion chromatograms (m/z 353.0873) of a chlorogenic acid standard, and the skin, pulp and arils, of a whole pomegranate.

These additional experiments suggest that North American pomegranates (grown and harvested during this time) do not contain any detectable amount of chlorogenic acid. It also suggests that the presence of chlorogenic acid in North American pomegranate juice may indicate the blending of other juices. To further understand the detection of chlorogenic acid in pomegranate varieties from different regions, a much broader mass spectrometric study is warranted.

EMRT 3.43_353.1448

Another EMRT of interest, 3.43_353.1448 was also investigated using the same workflow as described previously. The elemental composition was determined to be $C_{14}H_{26}O_{10}$. The extracted ion chromatograms of this m/z from the juice samples used in the study revealed it to be present in all pomegranate samples but at varying concentrations. For the juice blend (S6), it was present at a low level, as shown in Figure 9. However for the authentic juices, the levels were higher with the highest levels found in the authentic pomegranate juice (S2).

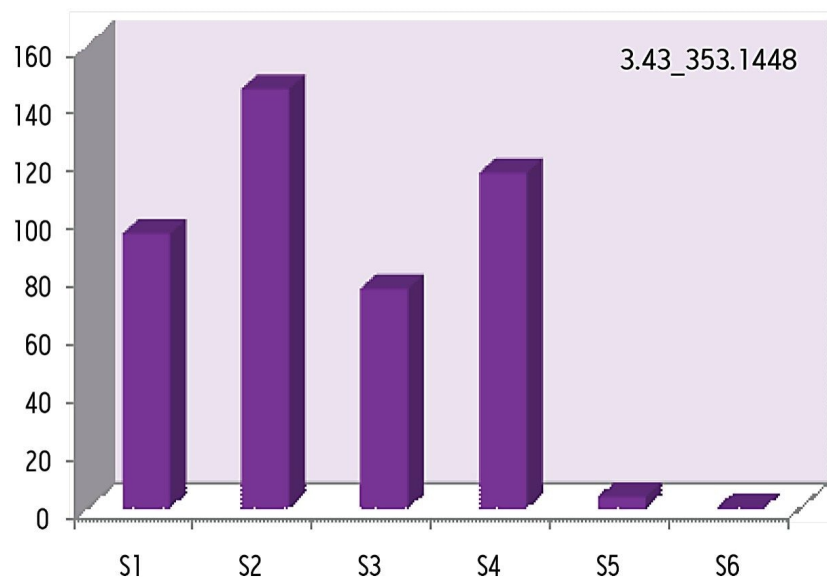


Figure 9. Variation of the levels of component 3.43_353.1448 in the pomegranate juice samples.

Extracted ion chromatograms of m/z 353.1448 in the whole fruit extracts (arils, pulp, and skin) shown in Figure 10A, revealed that this marker was only present in the arils, and that it was present in the arils of all three pomegranates, shown in Figure 10B.

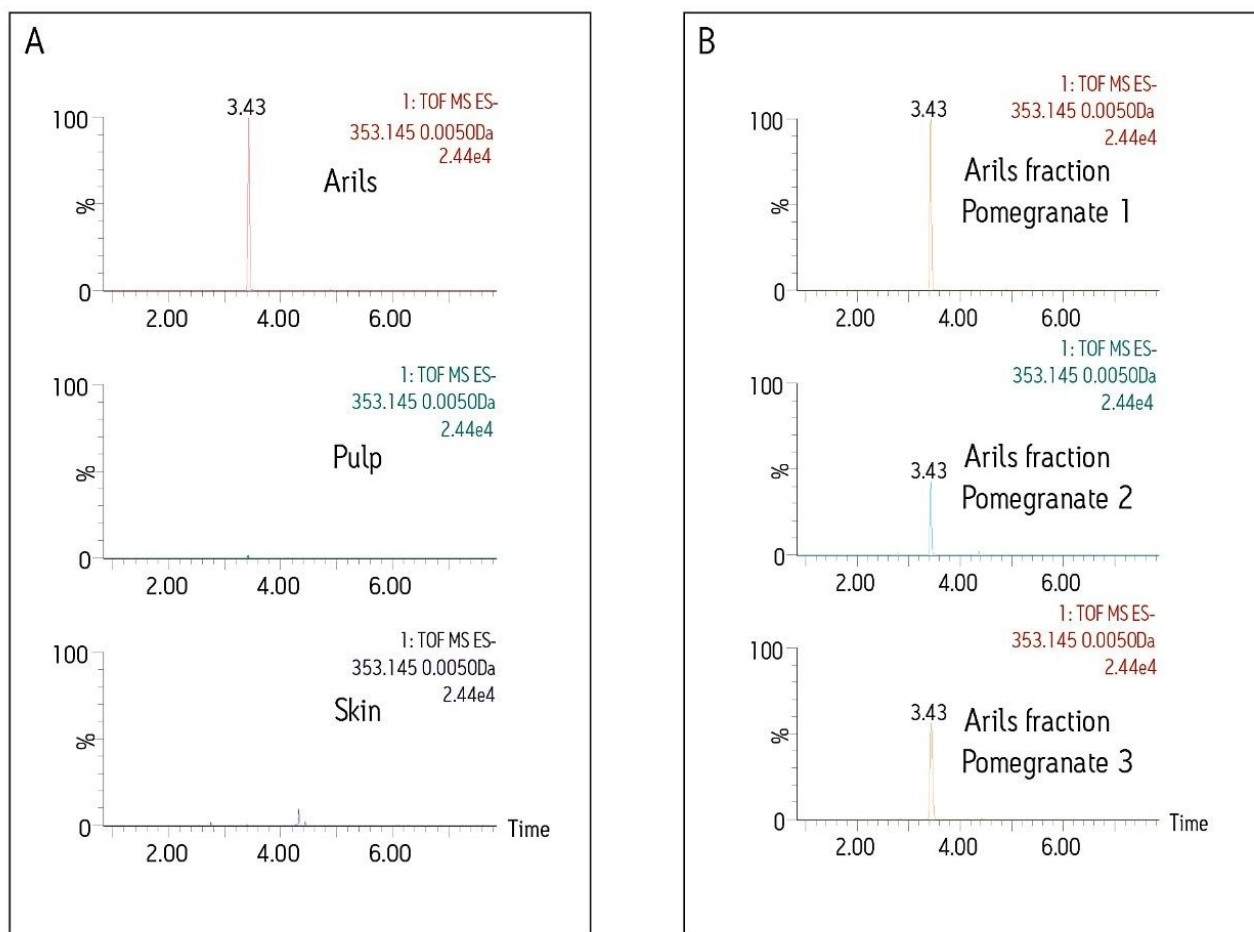


Figure 10A. Extracted ion chromatograms for marker 3.43_353.1448 in the arils, pulp and skin of a whole pomegranate.

Figure 10B. The marker was found in the arils of all pomegranates used in the study.

The uniqueness of this compound to pomegranate, and only within the arils of pomegranate suggests that it could be a valuable marker for the quality of pomegranate juice. However, additional experiments are required to identify this compound and study the seasonal, varietal, and geographical variations of the compound.

Summary of the results

Chlorogenic acid was absent in the authentic pomegranate juices analyzed in this study. Similarly it was not found in three whole fruit pomegranates. The adulterated samples used in this study, chlorogenic acid and two possible isomers were found to be present. This compound could, therefore be a potential marker compound for

determining pomegranate juice authenticity.

Conclusion

Economic adulteration of food and beverage products is a problem that has increased in magnitude because it has a lucrative outcome for unscrupulous members of the food manufacturing chains.

- Consumer demand for more exotic juices introduces analytical challenges for juice chemists.
- The ACQUITY UPLC System, ACQUITY UPLC PDA Detector, and Xevo G2 QTof MS, combined with a complete software workflow based on Markerlynx XS functionality, provide a powerful system solution for the analysis and determination of fruit juice authenticity in a research laboratory. Here these tools enabled the detection of compounds that have the potential to be used as indicators of a product's authenticity.
- The ACQUITY UPLC System provides high resolution chromatographic data for complex samples such as juice products.
- The ACQUITY UPLC PDA Detector and Xevo G2 QTof MS are complementary instruments for this type of analysis. This combination allows juice chemists to comprehensively research existing and new juice product prototypes in a fast-paced marketplace.
- MS^E functionality allowed the acquisition of low energy precursor (MS) and high energy product ions in a single run. The fragment data together with exact mass measurement provided added confidence and accuracy for structural elucidation.
- Intelligent analytical methods, such as the MarkerLynx XS profiling workflow presented in this application note, provide reliable and highly detailed information that can help in the process of food authentication.

References

1. Roberts MT. Cheaters Shouldn't Prosper and Consumers Shouldn't Suffer: The Need for Government Enforcement Against Economic Adulteration of 100% Pomegranate Juice and Other Imported Food Products.

Michael T. Roberts is Special Counsel for Roll Law Group PC. (2010).

2. Kearney AT and Grocery Manufacturers Association. Consumer Product Fraud: Deterrence and Detection, (2010).
3. Vai T, Jones PR, Sparkman OD . Rapid and unambiguous identification of melamine in contaminated pet food based on mass spectrometry with four degrees of confirmation. *J. Anal. Toxicol.* (2007) 31, 1319-1325.
4. Seeram NP et al. *In vitro* antiproliferative, apoptotic and antioxidant activities of punicalagin, ellagic acid, and a total pomegranate tannin extract are enhanced in combination with other polyphenols as found in pomegranate juice. *J Nutr Biochem.* 16, 6:360-7, 2005.
5. Mehta RE, Lansky EP. Breast cancer chemopreventive properties of pomegranate (*Punica granatum*) fruit extracts in a mouse mammary organ culture. *Eur J Cancer Prev.*13, 4:345-8, 2004.
6. Lansky EP et al. Pomegranate (*Punica granatum*) pure chemicals show possible synergistic inhibition of human PC-3 prostate cancer cell invasion across Matrigel. *Invest New Drugs.*23, 2:121-2, 2005.
7. Aviram M et al. Pomegranate juice consumption for 3 years by patients with carotid artery stenosis reduces common carotid intima-media thickness, blood pressure and LDL oxidation. *Clin Nutr.* 23, 3:423-33, 2004.
8. Zhang Y, Krueger D, Durst R, Lee R, Wang D, Seeram N , Heber D. International multidimensional authenticity specification (IMAS) algorithm for the detection of commercial pomegranate juice adulteration. *J. Agric. Food Chem.* 2009, 57, 2550-2557.
9. Eriksson L. Book "Multi- and Megavariable Data Analysis: Basic Principles and Applications", 2nd edition, 2008.
10. Poyrazoglu E, Gokmen V, Artuk N. Organic acids and phenolic compounds in pomegranates (*punica granatum*) grown in Turkey. *J. Food. Comp. Anal.* (2002) 15, 567-575.

Featured Products

ACQUITY UPLC System <<https://www.waters.com/514207>>

ACQUITY UPLC PDA eX Detector <<https://www.waters.com/10013843>>

Progenesis QI Software <<https://www.waters.com/134790655>>

MassFragment <<https://www.waters.com/1000943>>

720004010, August 2011

©2019 Waters Corporation. All Rights Reserved.

[Terms of Use](#)

[Privacy](#)

[Trademarks](#)

[Sitemap](#)

[Careers](#)

[Cookies](#)

[Cookie-Einstellungen](#)