Waters[™]

Nota de aplicación

Bioanalytical Method Development with UNIFI: Promoted Parameters

Robert S. Plumb, Stuart Chadwick, Jennifer Simeone, Paul D. Rainville

Waters Corporation



This is an Application Brief and does not contain a detailed Experimental section.

Abstract

The development of bioanalytical methodologies requires the evaluation of multiple chromatographic, sample preparation, and mass spectrometry parameters and conditions. The UNIFI Scientific Information System is equipped with a highly flexible interface, which allows the scientist to select specific parameters that need to be investigated.

Benefits

The promotable parameter function within the Waters UNIFI Scientific Information System facilitates the rapid acquisition of the data required to select the optimal LC and MS conditions for a bioanalytical assay.

Introduction

The development of bioanalytical methodologies requires the evaluation of multiple chromatographic, sample preparation, and mass spectrometry parameters and conditions. This often requires multiple iterations of changing experimental conditions, reviewing results, and performing follow-up experiments.

These tasks require a significant amount of manual input and are typically performed by expert or experienced scientists. The use of a simple templatedriven process allows the rapid, simple evaluation of all LC and MS parameters required to select the optimal method parameters. Previous LC-MS data systems did not have the flexibility to allow all of these parameters to be varied and tested in a simple straightforward manner.

The UNIFI Scientific Information System allows for the evaluation of many acquisition variables via the promotable parameters function. This approach allows the scientist to promote the experimental variable (e.g., capillary voltage) to be evaluated within the acquisition run list. The user can then vary the value of the parameter to be changed from injection to injection.



Figure 1. UNIFI Scientific Information System

Results and Discussion

The UNIFI Scientific Information System is equipped with a highly flexible interface, which allows the scientist to select specific parameters that need to be investigated. Once created, the sample list can be saved as a template for future use.

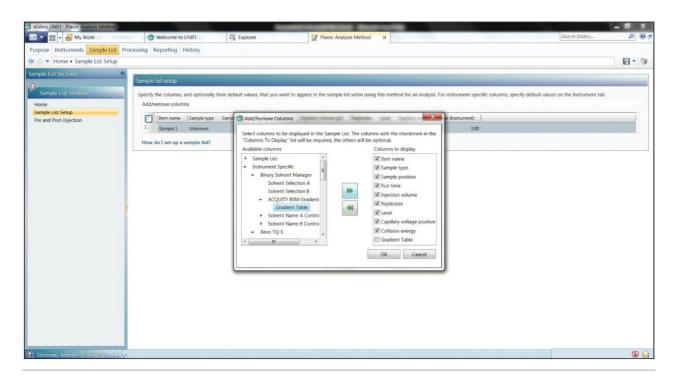


Figure 2. Creation of acquisition sample list with promotable parameters.

The ability to select and vary multiple experimental method parameters, column chemistry, mobile phases/ modifiers, capillary voltage, collision energy etc, in one simple data acquisition allows the scientist to acquire all the necessary data to identify the best LC-MS conditions quickly and efficiently.

The use of this approach is demonstrated in Figure 3 for the evaluation of the effect of changing the column temperature on analyte selectivity and sensitivity for the quantification of clopidogrel in extracted human plasma.

£.5	and the second							
					and the second		nple list controls	the second se
		atus:	Sample list run st		Stop	Pause	Start	nple tray: 1 🛛 🕘 📄
	list	start run o submit current sample	Click Start to		O	U	O	0000000
							mple list *	
							ld Delete	0000000
on status	Column temperature	Replicates Level	Injection volume (µL)	ion Run time (min)	Description Sample positi	Sample type Descri	Item name	E
	40 °C	1	10.00	3.50	40 1:A.1	Unknown 40	Column Temp Screen 1	1
	40 °C	1	10.00	3.50	40 1:A,2	Unknown 40	Column Temp Screen2	2
	40 °C	1	10.00	3.50	40 1:A3	Unknown 40	Column Temp Screen3	3
	50 °C	1	10.00	3.50	50 1:A4	Unknown 50	Column Temp Screen4	4
	50 °C	1	10.00	3.50			Column Temp Screen5	5
	50 °C		10.00	3.50			Column Temp Screen6	6
	60 °C			3.50			Column Temp Screen7	7
	60 °C			3.50			Column Temp Screen8	8
	60 °C	1	10.00	3.50	60 1:8.1	Unknown 60	Column Temp Screen9	9
	60 °C	1	10.00	3.50	60 1:8.1	Unknown 60	Column Temp Screen9	9

Figure 3. Evaluating the effect of a change in column temperature using UNIFI

Conclusion

The promotable parameter function within the Waters UNIFI Scientific Information System facilitates the rapid acquisition of the data required to select the optimal LC and MS conditions for a bioanalytical assay. The benefits to the scientist are:

- · Parameters to be varied can be selected and saved in a template for future use
- · Improved productivity
- · Greater number of parameters can be evaluated for optimal method selection
- · Reduced need for expert user

Featured Products

UNIFI Scientific Information System https://www.waters.com/134801648

Regulated Bioanalysis Platform Solution with UNIFI <https://www.waters.com/134613325>

720004286, February 2012

©2019 Waters Corporation. All Rights Reserved.