
Waters™

UPLC-MS/MS Method for the Quantification of Trastuzumab in Human Serum at the 5-nM Level Using Xevo TQD MS and ACQUITY UPLC H-Class System

Catalin E. Doneanu, Robert S. Plumb

Waters Corporation

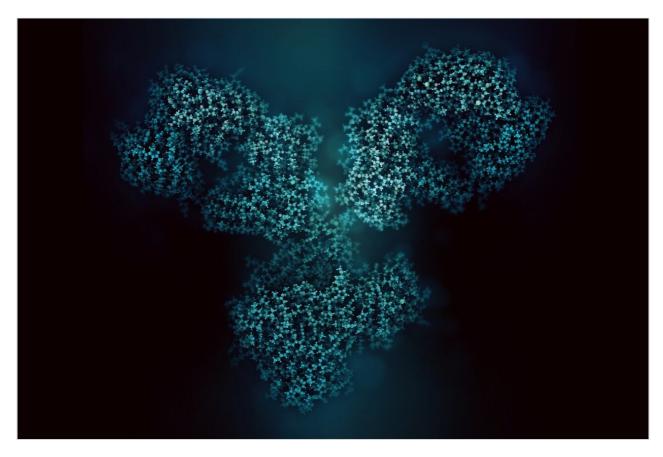

Abstract

In this application note, we report the development of a sensitive LC-MS/MS assay for the analysis of the signature peptide of trastuzumab with an assay sensitivity of 5 nM trastuzumab (0.75 μ g/mL) in human serum.

Benefits

This work demonstrates the capability of Xevo TQD to conduct bioanalysis of large protein molecules, as trastuzumab, a monoclonal antibody. Oasis micro-elution plates, the ACQUITY UPLC H-Class System, and an advanced tandem quadrupole mass spectrometer (Xevo TQD) were used for the development of a sensitive method for the quantification of trastuzumab in human serum digest. This application note addresses some critical challenges in the world of bioanalysis, such as developing a method to quantify protein molecules with desired sensitivity in a robust, reproducible, high-throughput LC-MS/MS system.

Introduction

Monoclonal antibodies (mAbs) comprise a new group of therapeutic compounds, which are used to treat cancer, auto-immune diseases, and systemic infections. HER2/neu receptor is over-expressed in about 25% of all breast cancer patients. Trastuzumab, as shown in Figure 1, directed against the HER2/neu receptor, is primarily used to treat certain breast cancers. It selectively binds with high affinity to the extracellular domain of the human epidermal growth factor receptor 2 protein, HER2. Trastuzumab is produced by recombinant DNA technology in a mammalian cell (Chinese hamster ovary) culture containing the gentamicin antibiotic. Trastuzumab is administered by intravenous infusions of 10 to 500 mg once every week. The compound demonstrated dose-dependent pharmacokinetics, with an average half-life of two and 12 days at the 10- and 500-mg dose levels, respectively. The volume of distribution of trastuzumab was approximately that of serum volume (44 mL/kg). At the highest weekly dose studied (500 mg), mean peak serum concentrations were 377 μ g/mL. A

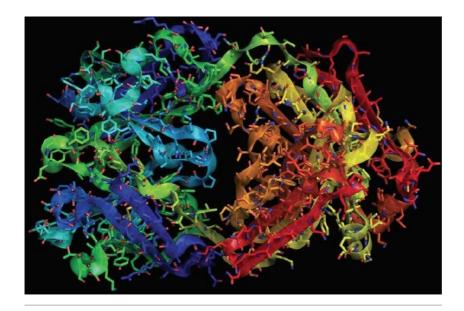


Figure 1. Molecular structure of trastuzumab.

Mass spectrometry is the analytical tool of choice for qualitative identification of mAbs. Quantification of mAbs in biological matrices utilizes enzyme-linked immune sorbent assay (ELISA), the most widely applied technique. However, LC-MS exhibits better specificity, and generates a better protein-specific charge envelope. In addition, structural changes in the molecule can be detected by the mass spectrometer, which is helpful in obtaining more insight in degradation patterns of mAbs, or to detect post-translational modifications. ELISA generates a result based on antibody binding properties, and does not reveal changes in the structure of mAbs. In this application note, we report the development of a sensitive LC-MS/MS assay for the analysis of the signature peptide of trastuzumab with an assay sensitivity of 5 nM trastuzumab (0.75 μ g/mL) in human serum.

Experimental

Sample Description

A stock solution of trastuzumab (a 150 kDa monoclonal antibody) was spiked with the internal standard (the $^{13}C^{15}N$ -isotopically labeled extended peptide *GR*FTISADTS*K*) and digested with trypsin to produce a stock solution containing 5 μ M digested trastuzumab and 5 μ M internal standard peptide (FTISADTS*K*). In parallel, 400 μ L of human serum was dispensed in 10 Eppendorf vials (40- μ L serum/vial) and digested with trypsin following the same procedure, to produce 400 μ L of human serum digest in each vial. The digestion protocol

involved sample denaturation (with 0.05% RapiGest at 80 °C for 10 min), disulfide bond reduction (in the presence of 20 mM dithiothreitol (DTT) at 60 °C for 60 min), cysteine alkylation (with 10 mM iodoacetamide (IAM) at room temperature for 30 min in the dark), and overnight digestion with porcine trypsin (25:1 (w/w) protein/ enzyme). Following digestion, 100 μ L of digested peptides were diluted 1:1 with a solution containing 4% H₃PO₄ and loaded onto an Oasis MCX mixed-mode μ Elution plate (P/N 186001830BA). Digests were washed with 200 μ L of 2% FA and 200 μ L of 5% methanol before being eluted with 2 x 50 μ L aliquots of 25% ACN in 2% NH₄OH (pH 10). The trastuzumab digest was spiked into the human serum digest (using more than 90% of the serum digest matrix for each dilution) at the following concentrations: 5, 10, 20, 50, 100, 200, and 500 nM trastuzumab.

LC-SRM Method Conditions

The analysis was performed on an ACQUITY UPLC H-Class System. A 10- μ L aliquot of the sample was injected onto an ACQUITY BEH130 C₁₈ 2.1 x 150 mm, 1.7 μ m column. The column temperature was maintained at 35 °C, with a flow rate of 0.3 mL/min. Mobile phases contained 0.1 % (v/v) formic acid (FA) in water (A), and 0.1% (v/v) FA in acetonitrile (B). Peptides were eluted with a linear gradient from 0% to 30% B over 10 min. The column effluent was monitored using a Xevo TQD Mass Spectrometer operated in selected reaction monitoring (SRM) positive ion electrospray mode. Four SRM transitions were monitored continuously throughout the LC-SRM assay using a dwell time of 40 ms: two SRMs monitored the endogenous signature peptide FTISADTS*K* from trastuzumab (485.2 \rightarrow 721.4 for peptide quantification; 485.2 \rightarrow 608.3 for peptide confirmation), while the other two SRM channels monitored the corresponding ¹³C¹⁵N-isotopically labeled internal standard peptide FTISADTS*K* (489.2 \rightarrow 729.4 for peptide quantification; 489.2 \rightarrow 616.3 for peptide confirmation).

Results and Discussion

Trastuzumab signature peptide (FTISADTSK) eluted with a retention time of 7.55 minutes, as shown in Figure 2. The data illustrates the injection of a 5 nM trastuzumab standard spiked in the human serum digest immediately following the analysis of human serum digest blank. This data shows very symmetrical peaks produced by the chromatography system that have a width at the base of approximately 4 seconds. The lower limit of quantification (LLOQ) for the assay was determined to be 5 nM (or 0.75 µg/mL) of trastuzumab in human serum, with an RMS signal to noise ratio of 27:1. A typical calibration obtained for the assay for the FTISADTSK signature peptide of trastuzumab is shown in Figure 3, with a correlation coefficient of 0.99326

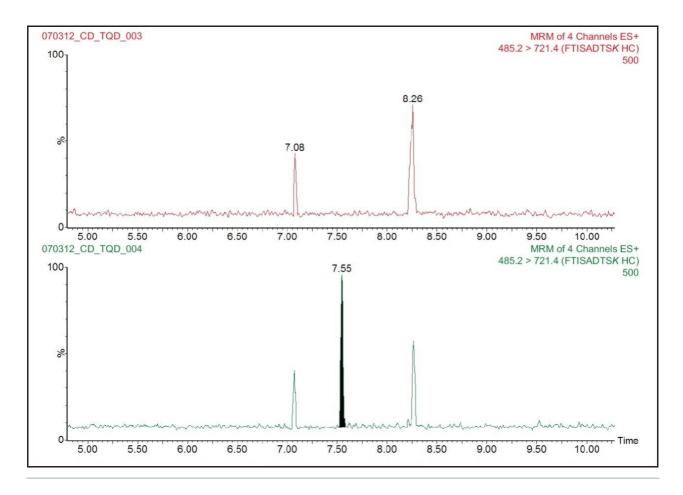


Figure 2. LC-SRM chromatogram of the 5-nM trastuzumab standard and the corresponding serum blank.

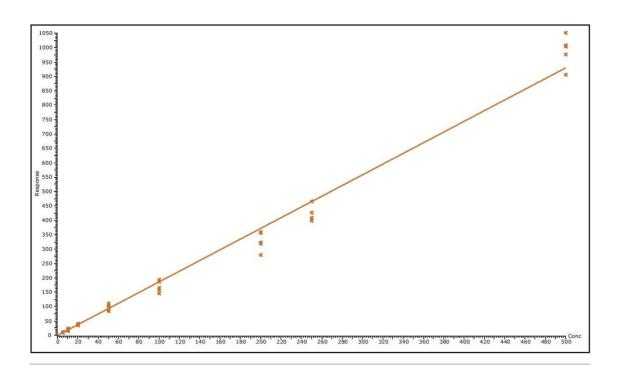


Figure 3. Representative calibration line for the LC-SRM quantification of trastuzumab.

Figure 4 shows the SRM chromatograms of a Solvent A blank run, following the injection of the highest standard tested (500 nM trastuzumab in human serum digest). We can see from this data that there is no discernable carryover in the blank chromatogram (where the baseline has been magnified) for the FTISADTS K peptide. The extremely low carryover exhibited by the ACQUITY UPLC H-Class System allows the full sensitivity of the Xevo TQD Mass Spectrometer to be exploited.

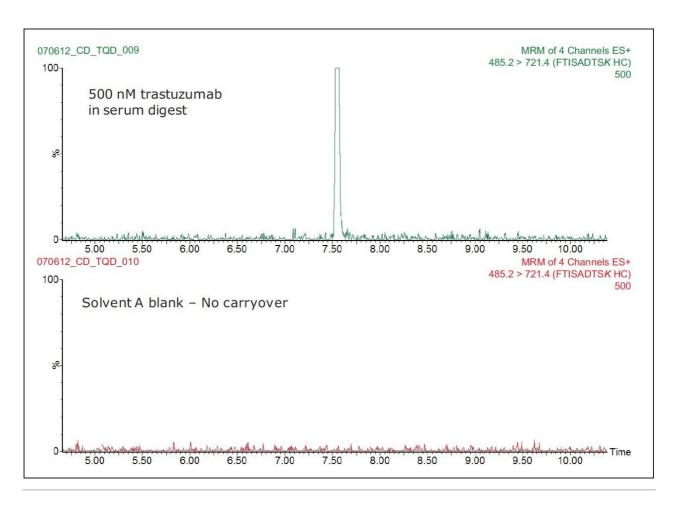


Figure 4. Carryover evaluation of the ACQUITY UPLC H-Class System.

Conclusion

- · A high-sensitivity method has been tested for the analysis of trastuzumab (150 kDa protein) in human serum digest using a signature peptide.
- · The level of quantification was determined to be 5 nM (0.75 μ g/mL).
- No significant carryover was detected, following the injection of the highest concentration standard tested (500 nM trastuzumab in human serum).

References

- 1. Brekke OH, Sandlie I. Nat. Rev. Drug Discov. 2003; 2, 52-62.
- 2. Carter P, Presta L, Gorman CM, Ridgway JB, Henner D, Wong WL, Rowland AM, Knotts C, Carver ME, Shepard HM. *Proc. Natl. Acad.* Sci. USA. 1992; 89, 4285-4289.
- 3. Hudis CA. N. Engl. J. Med. 2007; 357, 39-51.
- 4. Baughman TM, Graham RA, Wells-Knecht K, Silver IS, Tyler LO, Wells-Knecht M, Zhao Z. *Drug Metabolism and Disposition*. 2005; 33, 733-738.

Featured Products

ACQUITY UPLC H-Class PLUS System https://www.waters.com/10138533

Xevo TQD Triple Quadrupole Mass Spectrometry https://www.waters.com/134608730

720004423, July 2012

©2019 Waters Corporation. All Rights Reserved.