

Increasing the Abundance of Precursor Ions for Multiple Reaction Monitoring (MRM) Analysis by Atmospheric Pressure GC (APGC) Ionization

Dominic Roberts

Waters Corporation

This is an Application Brief and does not contain a detailed Experimental section.

Abstract

This application brief compares the ionization and fragmentation characteristics of pesticides using traditional electron ionization (EI+) GC-MS and APGC to improve MRM analysis of these compounds.

Benefits

Coupled with the Xevo TQ MS or Xevo TQ-S, APGC enables low-level quantification of persistent organic pollutants that have proved challenging to analyze using EI+ GC-MS systems.

Introduction

The Stockholm Convention (2004) is an international treaty that aims to eliminate or restrict the production

and use of certain persistent organic pollutants (POPs). Monitoring of the compounds on the banned list is required in a variety of environmental matrices. Several pesticides banned by the convention are difficult to analyze by traditional EI+ GC-MS due to significant levels of fragmentation. Therefore, this makes selection of a suitable precursor ion for MS/MS difficult. For multiple reaction monitoring (MRM) analysis, the ability to obtain an intense and specific precursor ion is critical in obtaining low detection limits.

A new ionization technique, Atmospheric Pressure GC (APGC) is presented here as an alternative. Ionization in APGC is analogous to atmospheric pressure chemical ionization (APCI) inasmuch as molecular or quasi-molecular ions are produced. APGC is a 'soft' ionization technique that results in lower fragmentation. The presence of strong molecular or quasimolecular ions provides ideal conditions for MS/MS analysis.



Results and Discussion

A Waters Xevo TQ-S coupled to a GC with an APGC Source was operated in MS Scan mode. A suite of pesticides was analyzed with any spectra obtained and compared against the NIST Mass Spectral Library. There are two possible ionization mechanisms, depending on the source conditions: nitrogen charge transfer, producing M^+ radical cations: or proton transfer, which produces $[M+H]^+$ ions depending on the source conditions. Dry source conditions will favor nitrogen charge transfer, whereas the presence of H^+ ions (e.g. from water or methanol) favor proton transfer.

Organochlorine insecticides, such as endosulfan and cyclodiene-type insecticides, such as aldrin, dieldrin, and endrin, have traditionally proven difficult to analyze in EI+ because of their extensive fragmentation. Due to this

fragmentation, the selection of a suitable precursor to product ion transition for MRM analysis is difficult.

Figure 2 shows the comparison between the spectrum for endosulfan taken from the NIST 08 Spectral Library and that obtained from APGC. Compared to the EI+ spectrum, the APGC spectrum shows a significant reduction in the fragmentation.

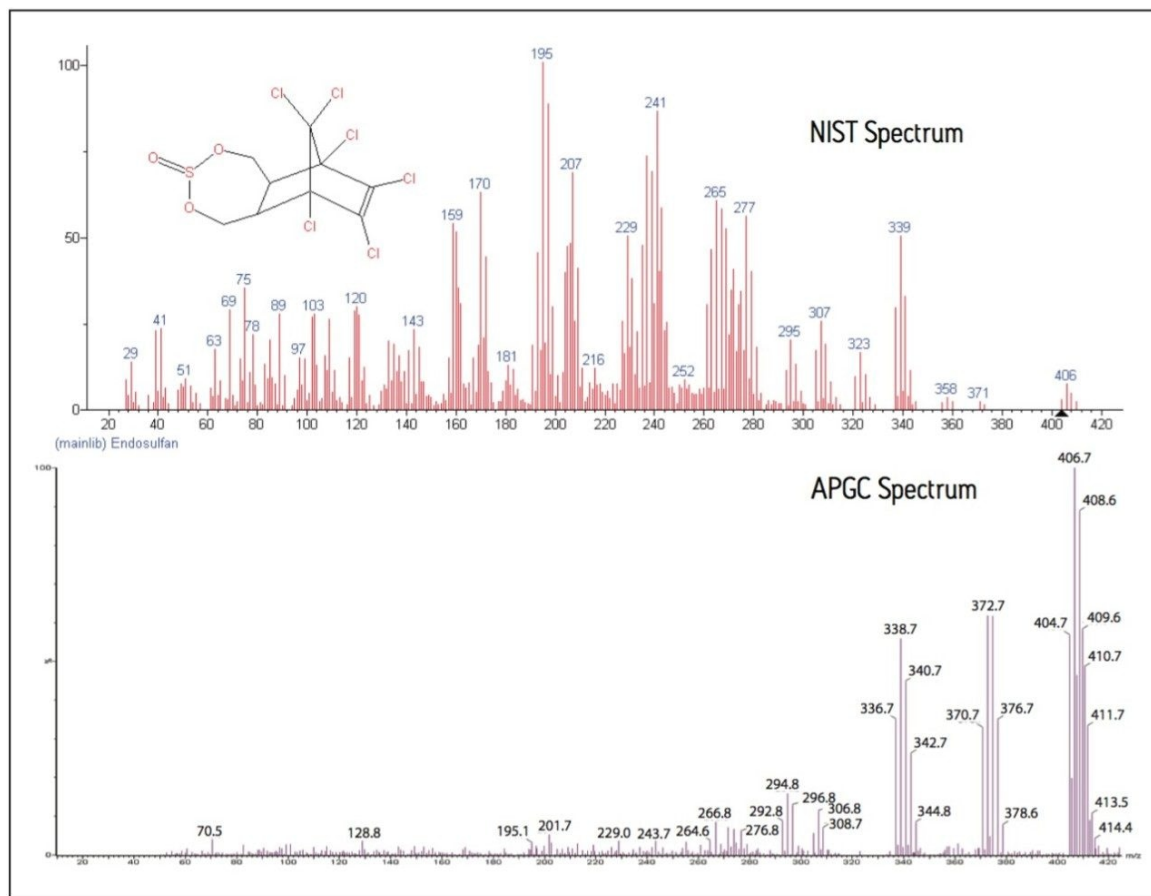


Figure 2. Comparison between the NIST library spectrum and the acquired spectrum of endosulfan

Using APGC, the predominant ion for endosulfan is m/z 407 $[M+H]^+$, rather than the fragment ion m/z 195 in the NIST spectrum. In addition, the ion signal is concentrated into a small number of ions, rather than spread across many fragments. The ions from the APGC spectrum are therefore much more suitable for the precursor ion selection required in MRM analysis. Good selection of the precursor ion is necessary for sensitive and specific MRM traces.

Figure 3 shows two MRM transitions of a low-level standard of endosulfan and also aldrin, dieldrin, and endrin. This demonstrates the application of this technique for the analysis of other traditionally difficult compounds.

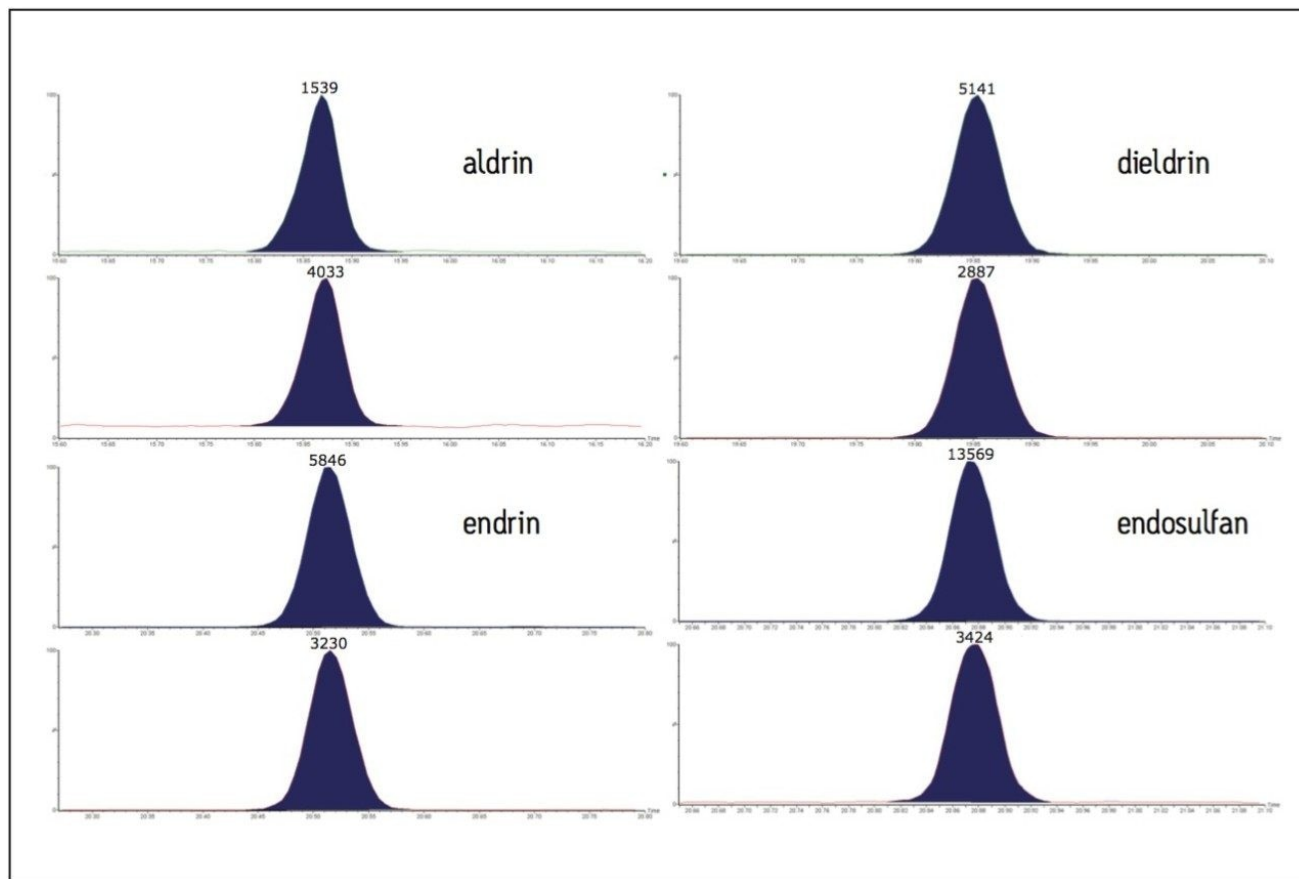


Figure 3. Two MRM transitions for aldrin, dieldrin, endrin, and endosulfan at 1 pg on-column.

Conclusion

- Waters' universal ionization sources, including APGC for Xevo and SYNAPT MS instruments facilitate the quick and simple coupling of GC to MS instruments.
- APGC is a soft ionization technique and therefore produces lower levels of fragmentation compared with traditional EI+. Depending on the source conditions, APGC typically produces spectra with strong radical cation molecular ions or protonated molecules.
- The abundant nature of these ions makes it possible to generate specific and sensitive MRM transitions for compounds that have been historically difficult to analyze.

- Coupled with the Xevo TQ MS or Xevo TQ-S, APGC enables low-level quantification of persistent organic pollutants that have proved challenging to analyze using EI+ GC-MS systems.

Featured Products

Xevo TQ-S <<https://www.waters.com/10160596>>

Waters Atmospheric Pressure Gas Chromatography (APGC) <<https://www.waters.com/10100362>>

720004031, December 2013

©2019 Waters Corporation. All Rights Reserved.

[Terms of Use](#)

[Privacy](#)

[Trademarks](#)

[Sitemap](#)

[Careers](#)

[クッキー](#)

[クッキ](#)

— [環境設定](#)