

USP Method Transfer of Donepezil Tablets from HPLC to UPLC

Mia Summers, Kenneth J. Fountain

日本ウォーターズ株式会社



Abstract

The USP compendial method for donepezil tablets was successfully transferred from HPLC to UPLC using

the Waters Column Selectivity Chart and ACQUITY UPLC Columns Calculator. Routine use, typical of a QC laboratory analyzing a formulated donepezil tablet sample, was evaluated on the ACQUITY UPLC BEH C₁₈ 1.7 µm column. Approximately 850 injections were achieved before peak splitting was evident and the method failed system suitability. Troubleshooting steps attributed the cause of failure to sample build-up on the column bed. Due to practical limitations in changes to the sample preparation, the method was transferred to an XBridge C₁₈ XP 2.5 µm column, where approximately 1600 injections were achieved. The method using the XP 2.5 µm column is approximately 80% faster than the HPLC method and results in a 92% savings in sample injected and solvent consumption. In cases where formulated sample is not directly compatible with the original compendial method, the use of XP 2.5 µm columns can provide method ruggedness while still providing significant sample throughput and solvent cost savings.

Benefits

- Updating USP Methods from HPLC to UPLC to increase analysis throughput and reduce solvent cost
- Increasing method robustness for complex formulations
- 80% decrease in analysis time, faster throughput for routine sample analysis
- 92% reduction in solvent usage and sample injected

Introduction

Compendial methods are often used in the analysis of generic drugs. Typically, methods are developed and submitted based on a specific formulation. However when the excipients are changed, the method specified in a USP monograph may be inadequate in eluting all components off of the column. The result can be deteriorating peak shape and premature method failure due to a build-up of poorly soluble excipients on the column.

Donepezil is a drug used to treat symptoms of dementia in Alzheimer's patients and is formulated in a tablet preparation. Here, we demonstrate the transfer of the USP compendial method for donepezil from HPLC to UPLC. Methods for assay and impurities analyses are sometimes combined to minimize the number of methods developed and submitted for regulatory approval. In this application, the transfer of the organic impurities method, which is a more complicated gradient separation, is demonstrated. Since impurity standards were not readily available, the transfer and routine use study is demonstrated using donepezil standard and tablets. A routine use study using conditions typical of a QC laboratory protocol is performed with the UPLC method and assay suitability criteria are evaluated to assess the long-term robustness of the method.

Experimental

Alliance 2695 HPLC conditions

Column:	XBridge C ₁₈ , 4.6 x 250 mm, 5 µm (L1), part number 186003117
Gradient:	25% B to 60% B over 10 min, hold for 30 min, return to 25% B in one min and re-equilibrate for 9 min
Flow Rate:	1.5 mL/min
Run Time:	50 min
Injection Volume:	20 µL

Acquity UPLC H-class system

Column:	ACQUITY UPLC BEH C ₁₈ 2.1 x 100 mm, 1.7 µm (L1), part number 186002352
Gradient:	25% B to 60% B over 2.5 min, hold for 7.5 min, return to 25% B in 0.25 min and re-equilibrate for 2.25 min
Flow Rate:	0.5 mL/min
Run Time:	12.5 min
Injection Volume:	1.7 µL
Column:	XBridge C ₁₈ <i>XP</i> , 2.1 x 100 mm, 2.5 µm (L1), part number 186006031
Gradient:	25% B to 60% B over 2 min, hold for 6 min,

	return to 25% B in 0.2 min and re-equilibrate for 1.8 min
Flow Rate:	0.63 mL/min
Run Time:	10 min
Injection Volume:	1.7 µL

HPLC and UPLC conditions

Mobile Phase:	A: 0.1% phosphoric acid in water, adjust to pH 6.5 with triethylamine B: acetonitrile
Diluent:	water:acetonitrile (3/1)
Needle Wash:	60:40 water:acetonitrile
Sample Purge:	60:40 water:acetonitrile
Seal Wash:	50:50 methanol:water
Column Temp.:	50 °C
Detection:	UV at 286 nm
Data Management:	Empower 3 CDS

USP System Suitability Criteria

Tailing Factor:	Not More Than (NMT) 1.5 USP Plate Count: Not Less Than (NLT) 40,000 plates
Replicate Injections:	NMT 2.0% RSD for donepezil peak (5 replicates)

Sample Preparation

Donepezil (1 mg/mL) in diluent: Waters Analytical Standard

Donepezil Tablets (1 mg/mL): Crushed tablets were weighed in a 50 mL volumetric flask and 25 mL diluent was added. The sample was sonicated for 15 minutes and made up to volume with diluent. The sample was mixed well, filtered through a 0.2 µm PTFE filter and centrifuged at 12,000 rpm for 5 minutes.

Results and Discussion

The USP method for donepezil describes sample preparation as ‘dissolve in diluent and sonicate if necessary’. When preparing the tablet sample according to the USP method, the final product is a solution with visible fine particulates. In order to render the sample clear and suitable for injection, the sample was further filtered through a 0.2 µm PTFE membrane and then centrifuged at 12,000 rpm for 5 minutes. Upon centrifugation, a small pellet was visible and the supernatant was carefully pipetted into a sample vial for injection.

The USP organic impurities method for donepezil describes the use of an L1 column and the suggested column is Kromasil C₁₈. Using the Waters Column Selectivity Chart, a more modern L1 column, XBridge C₁₈, was selected since this column chemistry is also available in smaller particle sizes. The USP compendial method was first run as described on an Alliance HPLC system using five replicate injections of donepezil standard and donepezil prepared tablet. System suitability criteria described in the monograph were monitored and found to be within specifications (Table 1).

The USP method was then transferred from HPLC to UPLC using the ACQUITY UPLC Columns Calculator. Scaling was performed accounting for particle size and the column was scaled to an ACQUITY UPLC BEH C₁₈ 1.7 µm column, which has the identical stationary-phase chemistry to the HPLC column (XBridge C₁₈). Five replicate injections of both donepezil standard and donepezil tablet were analyzed separately. System suitability criteria for donepezil, including %RSD for peak area, USP tailing and USP plate count were compared between HPLC and UPLC. A comparison of both systems is shown in Table 1, where the UPLC transferred method passes all criteria specified in the monograph. The run time of the UPLC method is 12.5 minutes compared to the 50-minute HPLC method (Figure 1), resulting in a 75% savings in analysis time and 92% savings in solvent consumption and sample injected.

	USP	HPLC	UPLC
Retention Time(min)	none	9.44	2.70
% RSD Area*	NMT 2.0	0.40	0.26
USP Tailing	NMT 1.5	0.71	0.74
USP Plate Count	NLT 40,000	57638	134196

* 5 replicate standard injections

Table 1. System suitability results comparing HPLC to UPLC for five replicate injections of donepezil standard.

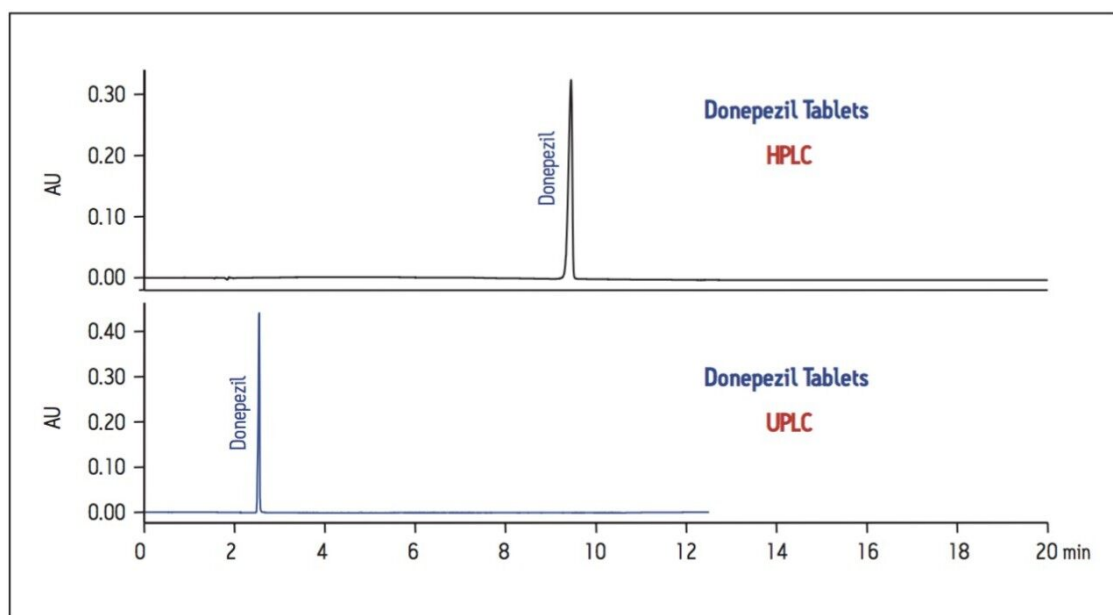


Figure 1. Chromatograms of donepezil tablet comparing HPLC to UPLC per the USP method.

(Note: the full 50-minute HPLC run time is not shown.)

Routine Use Study

Evaluation #1

In order to evaluate the effects of repeatedly analyzing a tablet drug formulation using a UPLC transferred USP method, a routine use evaluation was performed with the ACQUITY UPLC BEH C₁₈, 1.7 µm column using donepezil tablets.

Donepezil tablet samples were injected repeatedly using donepezil standard as a bracketing standard to emulate the process in a typical quality control (QC) laboratory. Mobile phase was prepared fresh daily to prevent bacterial growth. Twenty injections of donepezil tablet samples were made, along with five replicate injections of donepezil standard, and this cycle was repeated continuously until assay suitability

criteria no longer passed. Pressure, retention time, peak area, USP tailing and USP plate count were monitored throughout the study.

USP tailing remained within assay criteria throughout the study, however, after approximately 700 injections, the USP plate count began rapidly decreasing (Figure 2). At approximately 850 injections, the donepezil peak shape began to split (Figure 3) and the routine use study was stopped. Pressure remained stable throughout the study. The system was cleaned, mobile phases replaced and the column was washed. The column inlet and outlet frits were also replaced to determine if the poor peak shape could be attributed to particulate contamination, but the USP plate count still did not pass system suitability. These troubleshooting measures indicated that the UPLC column stationary phase had become contaminated by the poorly soluble excipients in the donepezil tablet formulation.

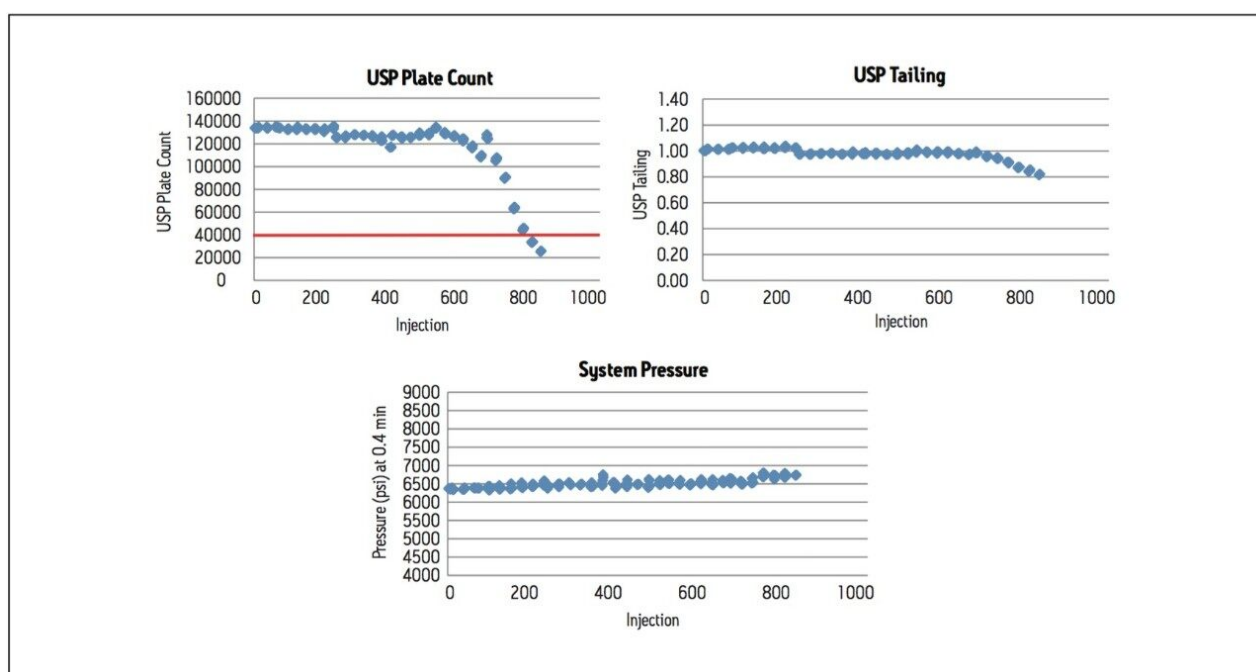


Figure 2. System suitability trend plots from routine use evaluation #1 (UPLC 1.7 μm column).

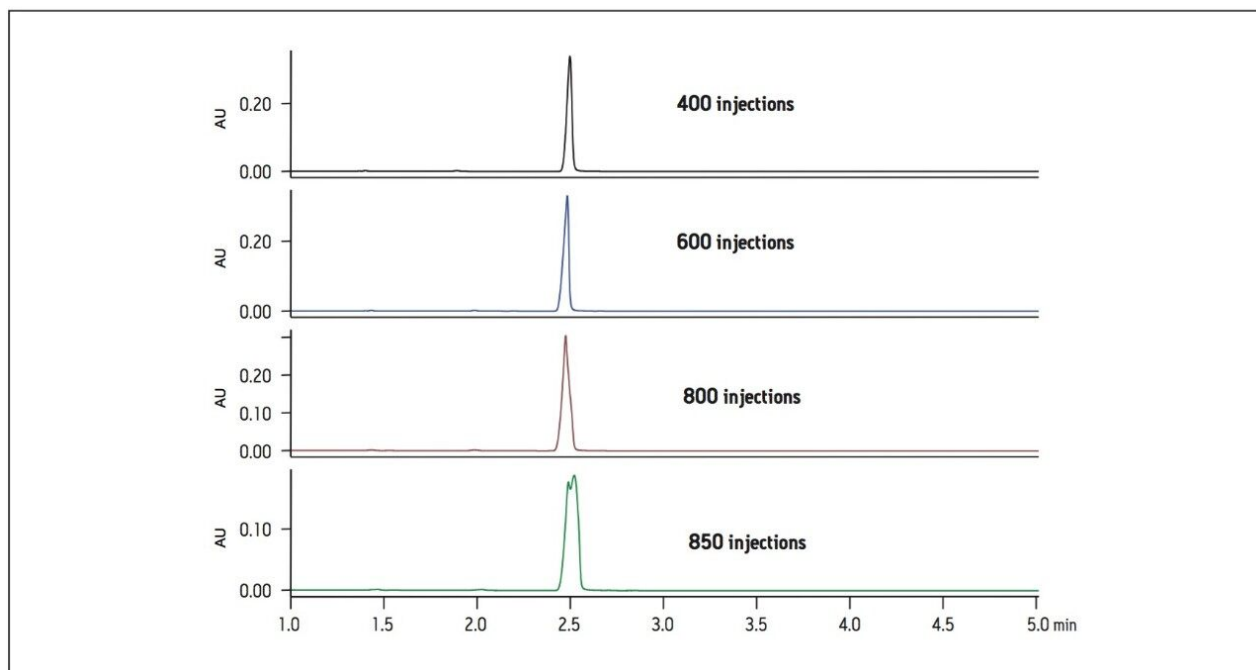


Figure 3. Chromatograms of donepezil standard from routine use evaluation #1 (UPLC 1.7 μ m column).

Evaluation #2

Sample preparation for formulated drug tablets is often limited due to time, cost and recovery concerns. For this reason, additional sample preparation steps were not pursued. Instead, the UPLC method using the ACQUITY UPLC 1.7 μ m column was transferred to an XBridge C₁₈ XP 2.5 μ m column using the ACQUITY UPLC Columns Calculator. Due to the larger particle size and subsequently lower backpressure, the method was run at a higher linear velocity, which resulted in a 10-minute method, an 80% savings in analysis time compared to the original 50-minute HPLC method.

A second routine use study was performed with the same repeating sample set containing donepezil standards and tablets, using the XP 2.5 μ m column. The results of this routine use study show USP plate count and USP tailing factor failing criteria after about 1600 injections (Figure 4). The routine use study was stopped at approximately 1700 injections, when the peak shape deterioration became evident (Figure 5).

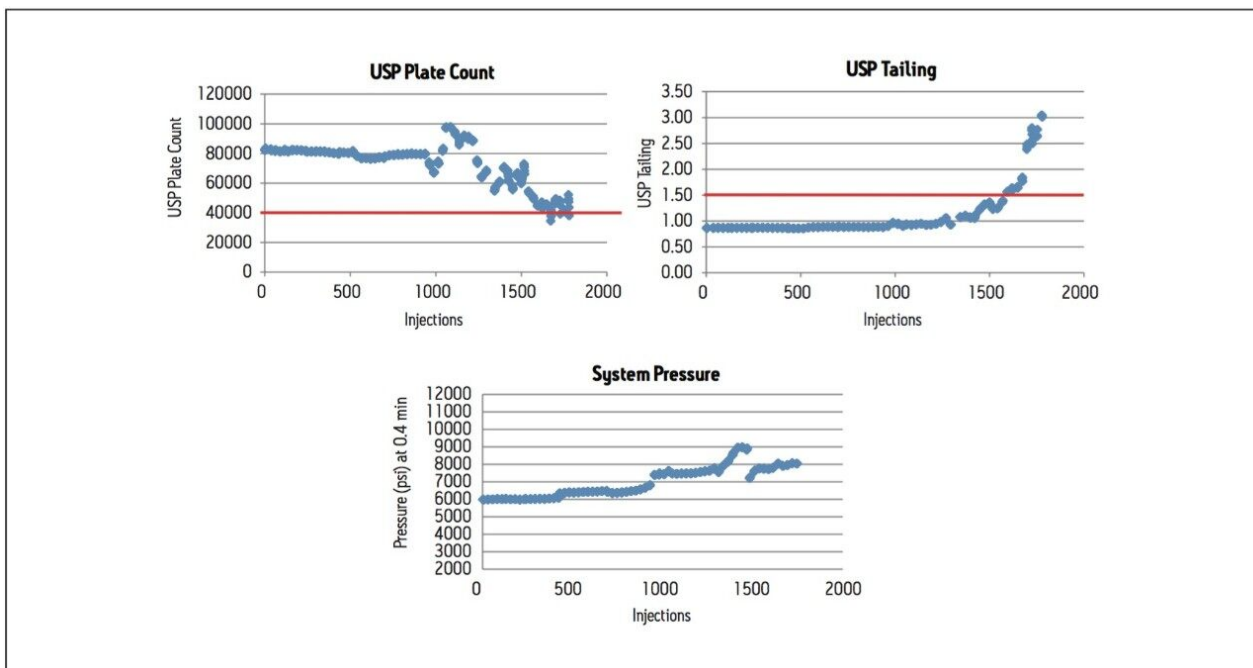


Figure 4. System suitability trend plots from routine use evaluation #2 (XP 2.5 μm column).

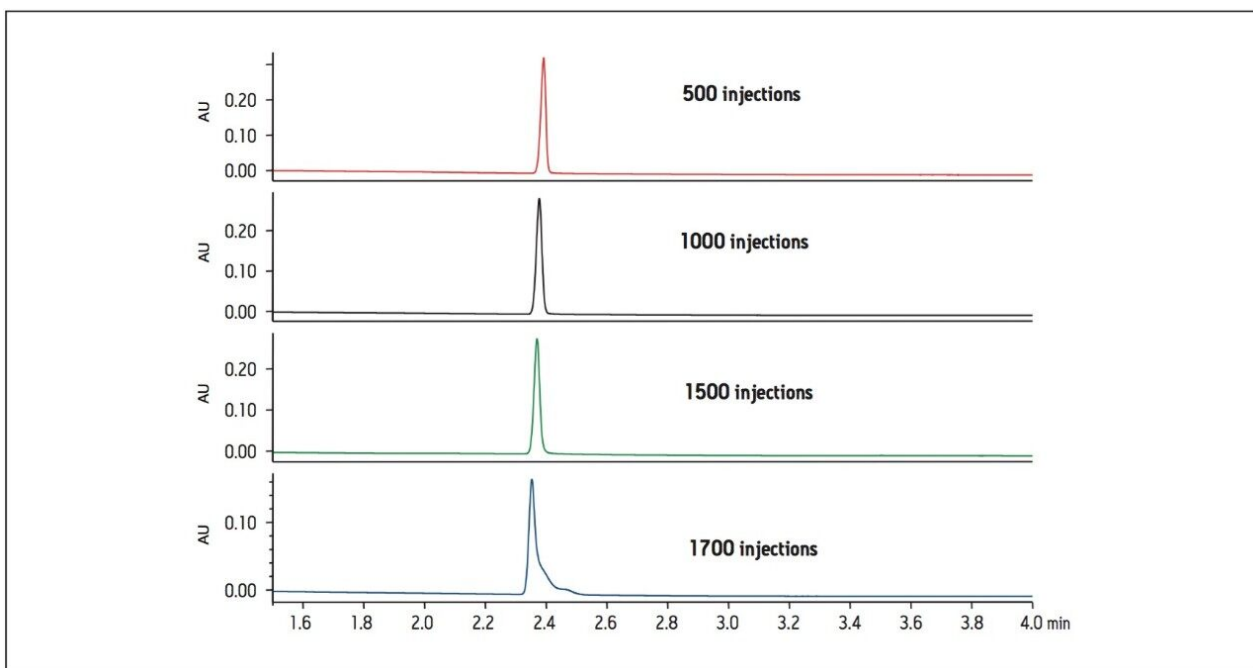


Figure 5. Chromatograms of donepezil standard from routine use evaluation #2 (XP 2.5 μm column).

Although the same formulation was analyzed, the XP 2.5 μm column resulted in twice as many injections compared to the 1.7 μm column. At 1600 injections, all system suitability criteria were still within

specification (Table 2). In the analysis of complex formulation matrices, there is limited removal of insoluble excipients using simplistic sample preparation procedures. This often results in an unavoidable build-up of sample components on the column. In the case of donepezil tablets, the use of an *XP* 2.5 μm column allowed for a greater number of injections, while still meeting the USP monograph system suitability requirements.

Routine Use Evaluation			
	USP Criteria	Start	1600 Injections
Retention Time(min)	none	2.35	2.27
%RSD Area*	NMT 2.0	0.49	0.32
USP Tailing	NMT 1.5	0.87	1.38
USP Plate Count	NLT 40,000	82472	44951

* 5 replicate standard injections

Table 2. System suitability results before and after 1600 injections from routine use evaluation #2 (*XP* 2.5 μm column).

Conclusion

The USP compendial method for donepezil tablets was successfully transferred from HPLC to UPLC using the Waters Column Selectivity Chart and ACQUITY UPLC Columns Calculator. Routine use, typical of a QC laboratory analyzing a formulated donepezil tablet sample, was evaluated on the ACQUITY UPLC BEH C₁₈ 1.7 μm column. Approximately 850 injections were achieved before peak splitting was evident and the method failed system suitability. Troubleshooting steps attributed the cause of failure to sample build-up on the column bed. Due to practical limitations in changes to the sample preparation, the method was transferred to an XBridge C₁₈ *XP* 2.5 μm column, where approximately 1600 injections were achieved. The method using the *XP* 2.5 μm column is approximately 80% faster than the HPLC method and results in a 92% savings in sample injected and solvent consumption. In cases where formulated sample is not directly compatible with the original compendial method, the use of *XP* 2.5 μm columns can provide method ruggedness while still providing significant sample throughput and solvent cost savings.

References

1. Jones M.D., Alden P., Fountain K.J., Aubin A. *Implementation of Methods Translation between Liquid Chromatography Instrumentation*, Waters Application Note [2010], Part Number 720003721EN.
2. USP Monograph. Donepezil Hydrochloride, USP35-NF30. The United States Pharmacopeial Convention, official from May 1, 2012.

Featured Products

ACQUITY UPLC H-Class PLUS System <<https://www.waters.com/10138533>>

Empower 3 Chromatography Data Software <<https://www.waters.com/513188>>

Alliance HPLC System <<https://www.waters.com/534293>>

Available for purchase online:

XBridge BEH C18 Column, 130Å, 5 µm, 4.6 mm X 250 mm, 1/pkg <
<https://www.waters.com/waters/partDetail.htm?partNumber=186003117>>

ACQUITY UPLC BEH C18 Column, 130Å, 1.7 µm, 2.1 mm X 100 mm, 1/pkg <
<https://www.waters.com/waters/partDetail.htm?partNumber=186002352>>

XBridge BEH C18 XP Column, 130Å, 2.5 µm, 2.1 mm X 100 mm, 1/pkg <
<https://www.waters.com/waters/partDetail.htm?partNumber=186006031>>

720004261, March 2013