Waters™

Application Note

Direct Analysis of Opioids and Metabolites from Whole Blood Using Ostro Sample Preparation Plates Combined with UPLC-MS/MS for Forensic Toxicology

Jonathan P. Danaceau, Erin E. Chambers, Kenneth J. Fountain

Waters Corporation



For forensic toxicology use only.

Abstract

The method presented in this study demonstrates the use of Ostro Sample Preparation Plates combined with UPLC-MS/MS for the analysis of 22 opioid compounds and metabolites of interest in whole blood samples. All compounds were analyzed in less than 5.5 minutes with complete resolution of all isobaric compound pairs. The use of Ostro Sample Preparation Plates allowed for rapid, in-well cell lysis and protein precipitation, followed by elution into a 96-well collection plate. This procedure resulted in improved throughput compared to protein precipitation in individual tubes, with the added benefit of removing endogenous phospholipid compounds. All analytes demonstrated good linearity over the entire calibration range, and the method was sensitive for reliable detection at the lowest curve points.

Benefits

- · Analysis of glucuronide metabolites without enzymatic hydrolysis
- · Comprehensive panel of 22 opiate and opioid analgesic compounds
- · Rapid and simple sample preparation compared to traditional LLE, SPE, or protein precipitation
- · Removal of endogenous phospholipids
- · Linear response for all analytes and metabolites

Introduction

The analysis of natural and synthetic opioid drugs continues to be an important aspect of forensic toxicology. A substantial percentage of arrests and/or deaths are attributed to the misuse or abuse of narcotic pain relievers such as oxycodone and hydrocodone, as well as the illegal opiate, heroin. Forensic laboratories often need to analyze whole blood specimens for the presence of different drugs to determine the precise cause of death, in cases of driving under the influence of drugs, or other criminal or research purposes. In the past, opioid analyses were typically conducted by GC/MS after first subjecting the samples to acid or enzymatic hydrolysis to liberate glucuronide metabolites. This step of using enzymatic hydrolysis to convert glucuronide metabolites to their free form adds time and expense to analysis, and complete and consistent hydrolysis is not always assured. With the advent of modern UPLC-MS/MS techniques, glucuronide metabolites can now be analyzed directly. The step of using enzymatic hydrolysis to death and consistent of modern uplaces.

Many sample preparation strategies have been used for whole blood analysis, including liquid-liquid extraction (LLE) and solid phase extraction (SPE). One of the simplest involves cell lysis followed by protein precipitation. The method presented in this study describes a rapid and straightforward sample preparation strategy using Ostro Sample Preparation Plates whereby whole blood samples can be pre-treated to lyse the cells, precipitated with acetonitrile, and eluted using a simple 96-well format. All sample pre-treatment is conducted within the wells of the Ostro Plate, without the need for centrifugation or sample transfer from individual tubes.

Following sample preparation, 22 opioid drugs and metabolites are subsequently analyzed by UPLC-MS/MS. Glucuronide metabolites are directly analyzed, eliminating the need for enzymatic or chemical hydrolysis. Calibration curves are linear with appropriate limits of detection easily reached.

Experimental

LC conditions

System:	ACQUITY UPLC
Column:	ACQUITY UPLC BEH C_{18} 2.1 x 100 mm, 1.7 μ m (p/n 186002352)
Column temp.:	30 °C
Injection volume:	10 μL
Flow rate:	0.4 mL/min
Mobile phase A:	0.1% formic acid in MilliQ water
Mobile phase B:	0.1% formic acid in ACN
Gradient:	Initial conditions were 2% B. The %B was increased to 52.8% over 6 minutes, then

returned to 2% over 0.5 minute. The system was allowed to re-equilibrate for 1.5 minutes. The entire cycle time was 8.0 minutes.

MS conditions

Mass spectrometer: Xevo TQD

Ionization mode: ESI positive

Acquisition mode: MRM (see Table 1 for transitions)

Capillary voltage: 1 kV

Collision energy (eV): Optimized for individual compounds (see Table

1)

Cone voltage (V): Optimized for individual compounds (see Table

1)

Data management

Waters MassLynx Software v4.1

Sample description

All compounds and internal standards (IS) were purchased from Cerilliant (Round Rock, TX).

Complementary, deuterated internal standards were used for all compounds with the exception of hydromorphone-3-glucuronide, codeine- 6-glucuronide, and norbuprenorphine-glucuronide. For these compounds, a deuterated IS with the most similar response was chosen as a surrogate.

A combined stock solution of all compounds (10 μ g/mL; 2.5 μ g/mL for fentanyl) was prepared in methanol. Working solutions were prepared daily with high standards and QCs in matrix (blood) and performing serial dilutions to achieve the desired concentrations. Calibrator concentrations ranged from 5 to 500 ng/mL for all analytes except fentanyl, which was prepared at 25% of the concentration of the other analytes (1.25 to 125.00 ng/mL). A combined internal standard stock solution (5 μ g/mL; 1.25 μ g/mL for fentanyl) was prepared

Sample preparation

Whole blood samples were prepared by adding 150 μ L of aqueous 0.1 M ZnSO₄/0.1 M NH₄CH₃COOH to the wells of an Ostro Pass-through Sample Preparation Plate. 50 μ L of whole blood was added to the ZnSO₄/NH $_4$ CH₃COOH solution and mixed briefly (5 s) to lyse the cells. 600 μ L of ACN containing internal standards was then added to the prepared samples. After vortexing for 3 minutes, the samples were eluted into a 96-well collection plate, evaporated to dryness under N₂, and reconstituted in 50 μ L of 0.1% formic acid in 2% ACN. 10 μ L was injected onto the LC-MS/MS system.

Results and Discussion

The 22 compounds and metabolites screened, listed in Table 1, constitute a comprehensive panel of natural opiate drugs, semi-synthetic opioids, and synthetic narcotic analgesic compounds. Most of the compounds are weak bases, with pKa values of approximately 8 to 9. They have a wide range of polarities, with LogP values ranging from -3.48 for morphine-3 β -d-glucuronide to 5.0 for methadone. MRM transitions used are also listed in Table 1. With the exception of tramadol and O-desmethyl tramadol, primary and confirmatory MRM transitions are listed along with their respective collision energies.

Comp	pound	RT	Formula	Molecular mass	MRM transitions	Cone voltage	Collision energy
1	Morphine-3β-D-glucuronide	1.21	C ₂₃ H ₂₇ NO ₉	461.17	462.1>286.1, 201.1	58	30, 52
2	Oxymorphone-3β-D-glucuronide	1.21	C ₂₃ H ₂₇ NO ₁₀	477.16	478.1>284.1, 227.1	46	28, 50
3	Hydromorphone-3β-D- glucuronide	1.34	C ₂₃ H ₂₇ NO ₉	461.17	462.1>286.1, 185.1	58	28, 56
4	Morphine	1.50	C ₁₇ H ₁₉ NO ₃	285.14	286.2>201.1, 165.1	54	28, 34
5	Oxymorphone	1.61	C ₁₇ H ₁₉ NO ₄	301.13	302.1>227.1, 242.1	44	28, 24
6	Hydromorphone	1.76	C ₁₇ H ₁₉ NO ₃	285.13	286.2>185.1, 157.1	66	32, 42
7	Codeine-6β-D-glucuronide	2.00	C ₂₄ H ₂₉ NO ₉	475.18	476.2>300.2, 165.2	60	36, 40
8	Dihydrocodeine	2.07	C ₁₈ H ₂₃ NO ₃	301.17	302.2>199.1, 128.1	52	34, 58
9	Codeine	2.14	C ₁₈ H ₂₁ NO ₃	299.15	300.2>215.2, 165.1	54	26, 38
10	Oxycodone	2.37	C ₁₈ H ₂₁ NO ₄	315.15	316.2>256.2, 241.1	44	26, 26
11	6-Acetylmorphone (6-AM)	2.41	C ₁₉ H ₂₁ NO ₄	327.15	328.2>165.1, 211.1	60	26, 36
12	O-desmethyl tramadol	2.46	C ₁₅ H ₂₃ NO ₂	249.17	250.2>58.0	26	18
13	Hydrocodone	2.50	C ₁₈ H ₂₁ NO ₃	299.15	300.2>199.1, 171.0	60	30,44
14	Norbuprenorphine-glucuronide	2.83	C ₃₁ H ₄₃ NO ₁₀	589.29	590.3>414.3, 101.0	70	34, 54
15	Tramadol	3.21	C ₁₆ H ₂₅ NO ₂	263.19	264.2>58.0	24	16
16	Normeperedine	3.58	C ₁₄ H ₁₉ NO ₂	233.10	234.1>160.1, 188.2	36	12, 18
17	Meperidine	3.60	C ₁₅ H ₂₁ NO ₂	247.16	248.2>174.1, 220.2	48	22, 20
18	Norbuprenorphine	3.77	C ₂₅ H ₃₅ NO ₄	413.26	414.3>101.0, 187.2	66	42, 34
19	Fentanyl	4.29	$C_{22}H_{28}N_2O$	336.22	337.2>188.2, 105.1	48	22,38
20	Buprenorphine	4.55	C ₂₉ H ₄₁ NO ₄	467.30	468.3>101.0, 396.3	72	40, 48
21	Propoxyphene	5.18	$C_{22}H_{29}NO_2$	339.30	340.3>266.2, 143.1	22	8, 32
22	Methadone	5.25	C ₂₁ H ₂₇ NO	309.20	310.2>105.0, 223.1	32	22, 28

Table 1. Chemical properties and MS conditions of test compounds.

Chromatography

A representative chromatogram of all compounds from a 50 ng/mL calibration standard is shown in Figure 1. Peak assignments can be found in Table 1. Using an ACQUITY UPLC BEH C_{18} 2.1 x 100 mm, 1.7 μ m Column, all analytes were analyzed in less than 5.5 minutes with a baseline separation between the critical isomer pairs of morphine-3-glucuronide and hydromorphone-3 glucuronide (compounds 1 and 3), morphine and hydromorphone (compounds 4 and 6), and codeine and hydrocodone (compounds 9 and 13). Total cycle time was 8.0 minutes.

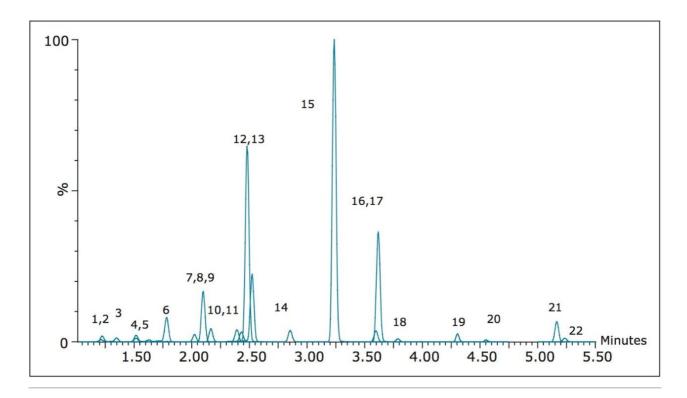


Figure 1. Chromatography of opiate and synthetic analgesic compounds. Peak assignments are listed in Table 1.

Recovery

For this application, evaporation of the organic eluate and reconstitution in a high aqueous solution (2% ACN) was necessary to prevent solvent effects that, otherwise, would interfere with the chromatography of the glucuronide metabolites. Figure 2 shows the average recovery of all compounds from whole blood using the Ostro Pass-through protocol detailed above. With the exception of the three earliest eluting glucuronide metabolites, all compounds demonstrated recoveries of 60% or greater, and the majority of compounds were recovered at 80% or greater.

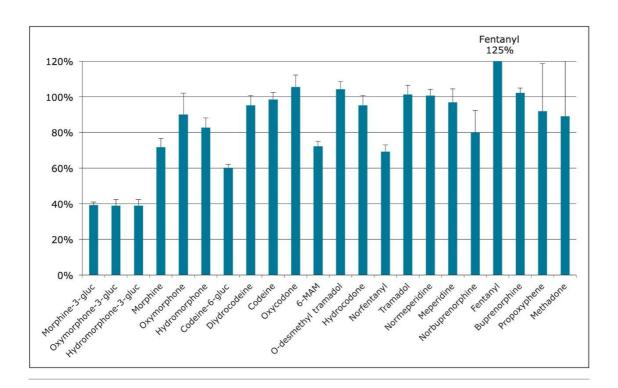


Figure 2. Recovery of opioid compounds from whole blood using Ostro Pass through Sample Preparation Plates. Bars represent the mean recovery from whole blood samples (N=4).

Linearity and sensitivity

The whole blood extraction method described herein was evaluated for linearity. Calibration standards were prepared in urine at concentrations ranging from 5 to 500 ng/mL (1.25 to 125.00 ng/mL for fentanyl). Table 2 summarizes the R² values, % deviations, and %CVs for all of the compounds. The average deviation of all calibration points from the curve was less than 2% for all compounds, and mean %CV values were less than 10% for all but three compounds. Individually, >93% of all calibrators were within 15% of their nominal concentration and >95% of the %CVs for individual calibration points (N=3) were less than 15%. Individual R values were all greater than 0.973, and all but 2 were greater than 0.98. In addition to the good linearity seen over the calibration range, all compounds demonstrated excellent sensitivity. At 5 ng/mL, the UPLC-MS/MS signal for oxymorphone-3-glucuronide, the least sensitive compound, was at least 20x greater than that of a blank extracted whole blood sample. In most cases, the signal for this low calibrator well exceeded 100x the method blank signal.

			Accuracy		%CV	
Compound		R ²	Mean	S.D.	Mean	S.D.
1	Morphine-3-β-d-glucuronide	0.985	99.7	4.9	9.6%	4.6%
2	Oxymorphone-3-b-d-glucuronide	0.983	100.7	4.7	8.4%	6.6%
3	Hydromorphone-3-b-d-glucuronide	0.986	100.8	8.3	8.2%	3.8%
4	Morphine	0.986	101.0	7.4	10.0%	2.9%
5	Oxymorphone	0.989	98.9	6.5	5.7%	3.3%
6	Hydromorphone	0.988	99.4	8.1	4.6%	2.1%
7	Codeine-6-β-d-glucuronide	0.973	99.8	13.5	6.5%	4.2%
8	Dihydrocodeine	0.984	99.8	11.4	7.0%	2.2%
9	Codeine	0.979	101.1	14.1	4.3%	2.2%
10	Oxycodone	0.986	99.0	12.4	4.4%	3.6%
11	6-Acetylmorphone (6-AM)	0.984	100.4	7.1	11.7%	3.4%
12	O-desmethyl Tramadol	0.990	100.3	6.7	5.2%	2.6%
13	Hydrocodone	0.990	100.5	6.8	5.5%	4.8%
14	Norbuprenorphine-glucuronide	0.989	101.0	7.4	11.1%	6.9%
15	Tramadol	0.988	100.5	10.2	3.4%	1.9%
16	Normeperedine	0.995	100.4	4.9	4.2%	2.6%
17	Meperidine	0.994	100.3	6.4	4.2%	2.3%
18	Norbuprenorphine	0.989	100.5	7.6	6.6%	4.4%
19	Fentanyl	0.992	99.6	5.8	5.2%	2.3%
20	Buprenorphine	0.994	100.3	5.5	5.5%	2.3%
21	Propoxyphene	0.990	100.5	7.5	4.2%	1.7%
22	Methadone	0.994	100.3	6.3	2.8%	0.4%

Table 2. Accuracy and coefficients of variation (%CV) from opiate calibration curves prepared using a simple sample dilution protocol. The concentrations of fentanyl and norfentanyl were 1/4 that of the other compounds.

Conclusion

The method presented in this study demonstrates the use of Ostro Pass-through Sample Preparation Plates combined with UPLC-MS/MS for the analysis of 22 opioid compounds and metabolites of interest in whole

blood samples. All compounds were analyzed in less than 5.5 minutes with complete resolution of all isobaric compound pairs. The use of Ostro Pass-through Sample Preparation Plates allowed for rapid, in-well cell lysis and protein precipitation, followed by elution into a 96-well collection plate. This procedure resulted in improved throughput compared to protein precipitation in individual tubes, with the added benefit of removing endogenous phospholipid compounds. All analytes demonstrated good linearity over the entire calibration range, and the method was sensitive for reliable detection at the lowest curve points.

References

- 1. Goldberger BA, Cone EJ. Confirmatory tests for drugs in the workplace by gas chromatography-mass spectrometry. *Journal of Chromatography A.* 1994; 674(1-2): 73-86.
- Wang P, et al. Incomplete recovery of prescription opioids in urine using enzymatic hydrolysis of glucuronide metabolites. *Journal of Analytical Toxicology*. 2006; 30(8): 570-575.
- 3. Gustavsson E, et al. Validation of direct injection electrospray LC-MS/MS for confirmation of opiates in urine drug testing. *Journal of Mass Spectrometry.* 2007; 42(7): 881-889.
- 4. Murphy CM, Huestis MA. LC-ESI-MS/MS analysis for the quantification of morphine, codeine, morphine-3-β-D-glucuronide, morphine-6-β-Dglucuronide, and codeine-6-β-D glucuronide in human urine. *Journal of Mass Spectrometry.* 2005; 40(11): 1412-1416.
- 5. Edinboro L, Backer RC, Poklis A. Direct analysis of opiates in urine by liquid chromatography-tandem mass spectrometry. *Journal of Analytical Toxicology.* 2005; 29(7): 704-710.
- 6. French D, Wu A, Lynch K. Hydrophilic interaction LC-MS/MS analysis of opioids in urine: significance of glucuronide metabolites. *Bioanalysis*. 2011; 3(23): 2603-2612.

Featured Products

ACQUITY UPLC System https://www.waters.com/514207

Xevo TQD Triple Quadrupole Mass Spectrometry https://www.waters.com/134608730

MassLynx MS Software https://www.waters.com/513662

Available for Purchase Online

ACQUITY UPLC BEH C18 Column, 130Å, 1.7 µm, 2.1 mm X 100 mm, 1/pkg < https://www.waters.com/waters/partDetail.htm?partNumber=186002352>

720004673, November 2014

©2019 Waters Corporation. All Rights Reserved.