


Nota applicativa

Gas-Phase Separation of Benzocaine Protonation Site Isomers and Phenylalanine Using Travelling-Wave Ion Mobility MS

Jonathan P. Williams, Martin Palmer, Jasper Boschmans, Filip Lemière, Frank Sobott

Waters Corporation, Biomolecular and Analytical Mass Spectrometry Group, Department of Chemistry, University of Antwerp, Centre for Proteomics, University of Antwerp

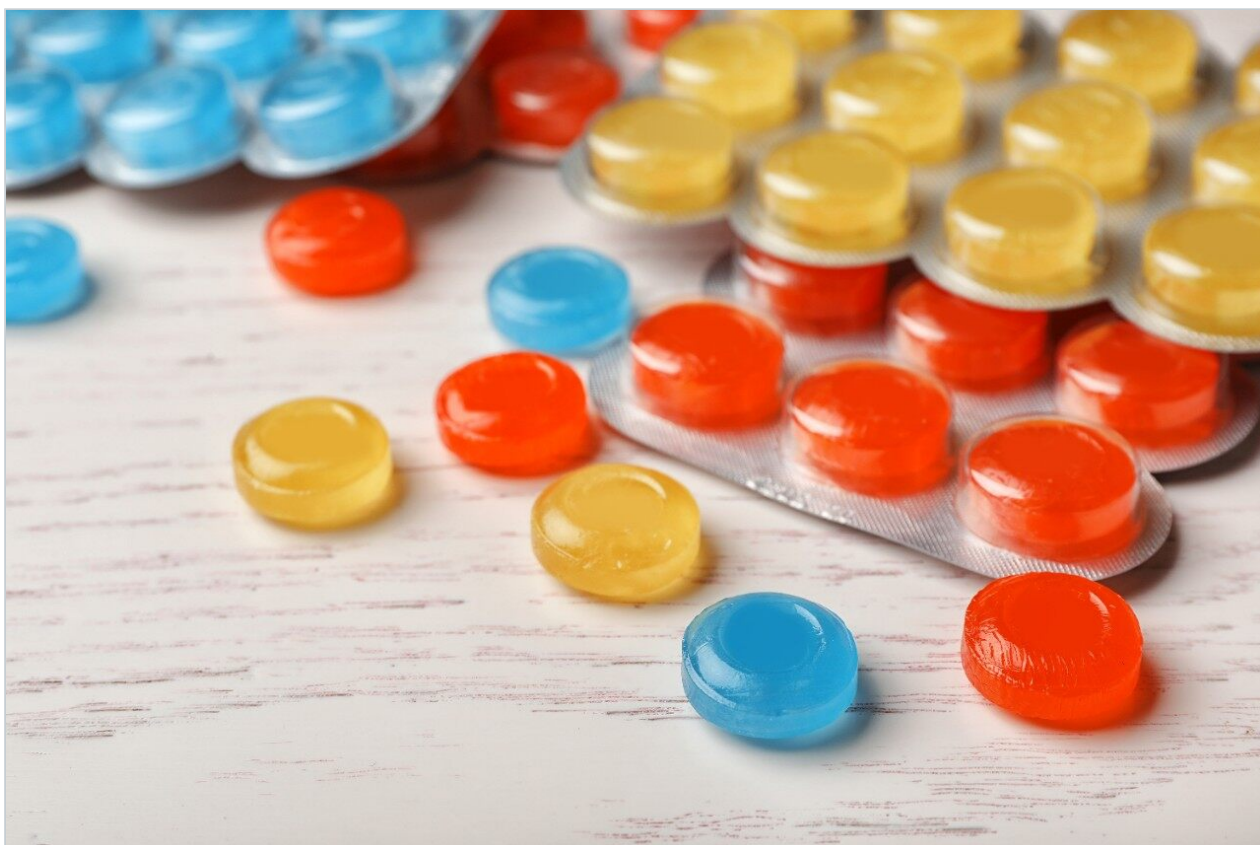

Abstract

In this application note, the SYNAPT G2-Si HDMS Travelling-Wave (T-Wave) Ion Mobility Mass Spectrometer (IMMS) has been used to separate the structural isomers benzocaine and phenylalanine.

Benefits

- The combination of ion mobility-MS to screening protocols will augment other metabolic studies and applications whereby interferences may be present
- Alternative ion mobility gases may provide a better separation of isomeric/isobaric species

Introduction

As part of the newborn metabolic screening protocol, the early identification of babies at risk of a metabolic disorder allows for the correct medical treatment and management of selected inherited disorders. A particularly effective method for the analysis of certain metabolites from dried blood spots, which may indicate a metabolic disorder, is electrospray ionisation combined with tandem mass spectrometry.¹ A number of inherited diseases result in the disruption of the metabolism and transformation of amino acids.

For example, approximately 1 in 12,000 children in the UK is born with an inherited metabolic disorder called phenylketonuria (PKU). PKU, a deficiency in phenylalanine hydroxylase inhibits the conversion of phenylalanine to tyrosine, with an accumulation of phenylalanine and a decrease in tyrosine. Thus, the phenylalanine to tyrosine ratio is useful in diagnosing PKU. If phenylketonuria is not detected and treated, the levels of phenylalanine in the child's blood will increase resulting in brain damage and mental retardation.

Any change in the way blood samples are collected prior to submission for MS analysis can adversely affect the measured concentrations of the targeted metabolites being measured. This was recently highlighted in the screening protocol for PKU whereby the hospital reported an increase in PKU abnormal.¹ The abnormally high levels were due to a contamination issue that was identified as an interference with benzocaine. The midwives used alcohol swabs which contained benzocaine to clean the skin prior to taking a blood spot via a heel prick of the newborns. Benzocaine is a structural isomer of phenylalanine and confirmed as the source of the PKU false positives.

The SYNAPT G2-Si HDMS Travelling-Wave (T-Wave) Ion Mobility Mass Spectrometer (IMMS) has been used to separate the structural isomers benzocaine and phenylalanine. Benzocaine has two protonation site isomers (protomers) that are detected at different mobility drift times to one another.^{2,3} The individual drift times of these protomers are importantly different to the ion mobility of phenylalanine.

Experimental

Sample preparation

Benzocaine (Sigma-Aldrich, St Louis, MO) and Phenylalanine (Sigma-Aldrich) stock solutions were prepared at 1 mg/mL and 0.4 mg/mL (MeOH) respectively. The samples were further diluted to 0.5 ng/ μ L (MeOH) and mixed prior to analysis by direct infusion MS.

Mass spectrometry

MS system:	SYNAPT G2-Si
Ionization mode:	ESI positive
Capillary voltage:	2.5 kV
Cone voltage:	20 V
Source temp.:	110 °C
Desolvation temp.:	250 °C

The ion signal was attenuated such that only ~5% of the ions were transmitted to the ion mobility cell.

Travelling wave ion mobility

N₂ parameters

T-Wave ion mobility cell: N₂ pressurized at a flow rate of 90 mL/min

T-Wave velocity: 750 m/s

T-Wave amplitude: 27 V

CO₂ parameters

T-Wave ion mobility cell: CO₂ pressurized at a flow rate of 65 mL/min

T-Wave velocity: 1000 m/s

T-Wave amplitude: 40 V

Results and Discussion

Benzocaine has two protomers that are detected at different mobility drift times, see Figure 1. The individual drift times of these protomers are importantly different to the ion mobility of phenylalanine. Protonation on either the amine nitrogen or the carbonyl oxygen generates protonation site isomers that interact differently with the mobility drift gas.

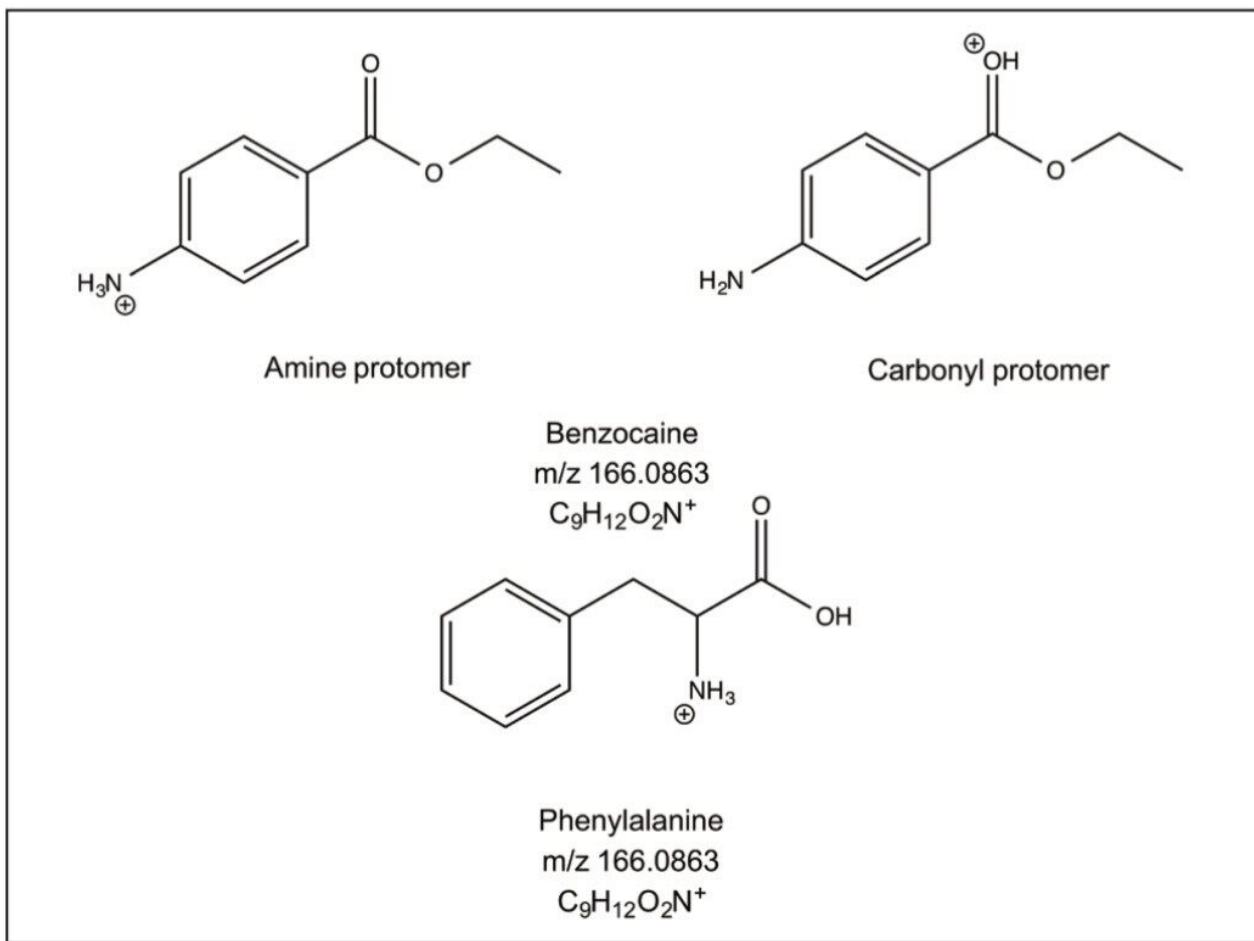


Figure 1. Possible protonation sites of benzocaine and phenylalanine.

As a consequence of the different sites of protonation, infusion of benzocaine into the T-Wave ion mobility section of the instrument results in two resolved ion mobility peaks detected at different drift times (data not shown). Addition of the structural isomer phenylalanine to a solution of benzocaine results in three components being separated and detected using ion mobility as shown in Figure 2. The drift times of the mobility separated m/z 166 ions are shown using N_2 mobility drift gas (Figure 2A) and CO_2 mobility drift gas (Figure 2B).

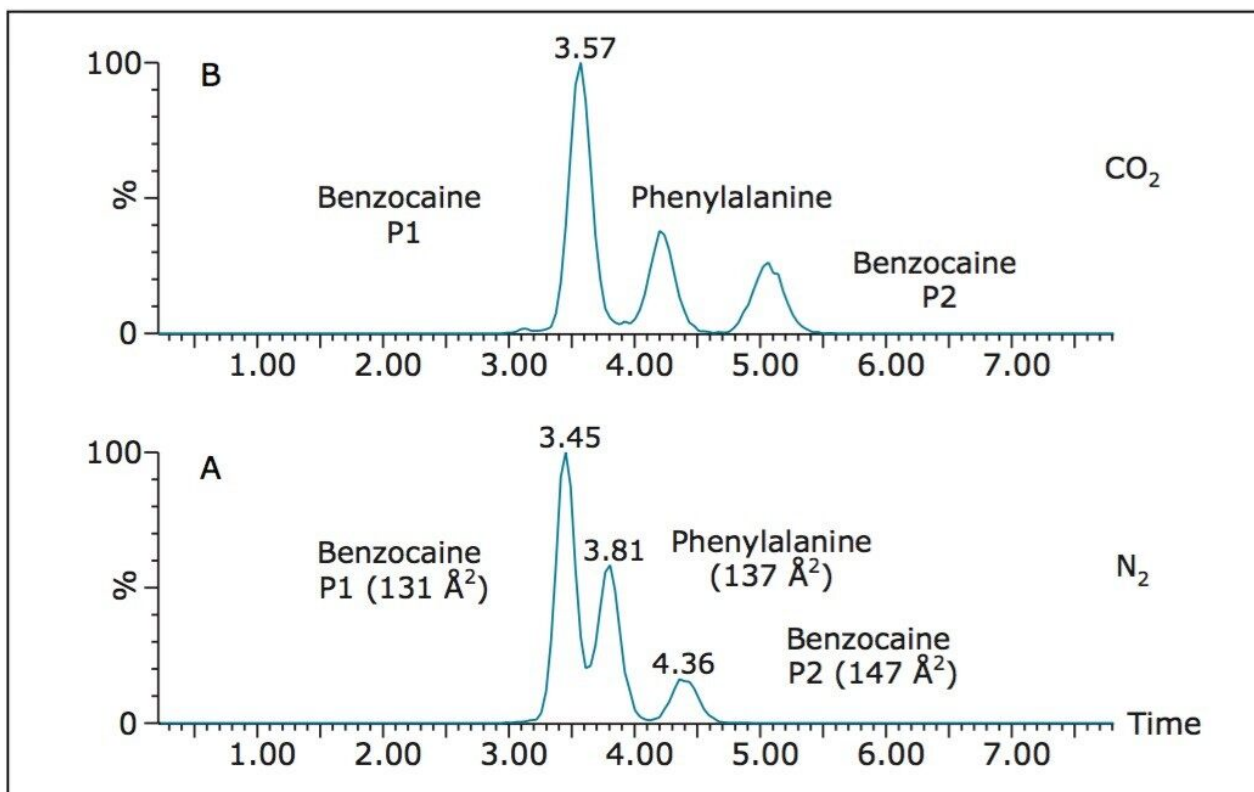


Figure 2. Ion mobility drift times (ms) for m/z 166 for both benzocaine protonation site isomers and phenylalanine obtained in N₂ mobility drift gas (A) and CO₂ mobility bath gas (B).

The T-Wave ion mobility rotationally-averaged collision cross-sections measured in N₂ for phenylalanine, and the protomers of benzocaine were 137 Å², 131 Å², and 147 Å², respectively. The results show that one of the protomers of benzocaine has a much greater interaction with the mobility gases of N₂ and CO₂ than the other protomer and phenylalanine. Following mobility separation, the ion species were fragmented by applying a potential difference of 15 V between the mobility and transfer T-Wave section of the instrument. By combining the mass spectra over the individual peaks in the drift times, tandem mass spectra were independently obtained. Figure 3A shows the MS/MS spectrum of the peak centred around 3.45 ms for one of the protomers of benzocaine. Figure 3B shows the MS/MS spectrum of the second peak centred around 4.36 minutes for the other protomer of benzocaine. Figure 3C shows the MS/MS spectrum of the peak centred around 3.81 minutes and is consistent with fragmentation of phenylalanine. The resulting product ions obtained, and abundances for fragmentation of benzocaine, are due to different fragmentation pathways as a direct result of the different positions of protonation, as shown in Figure 3.

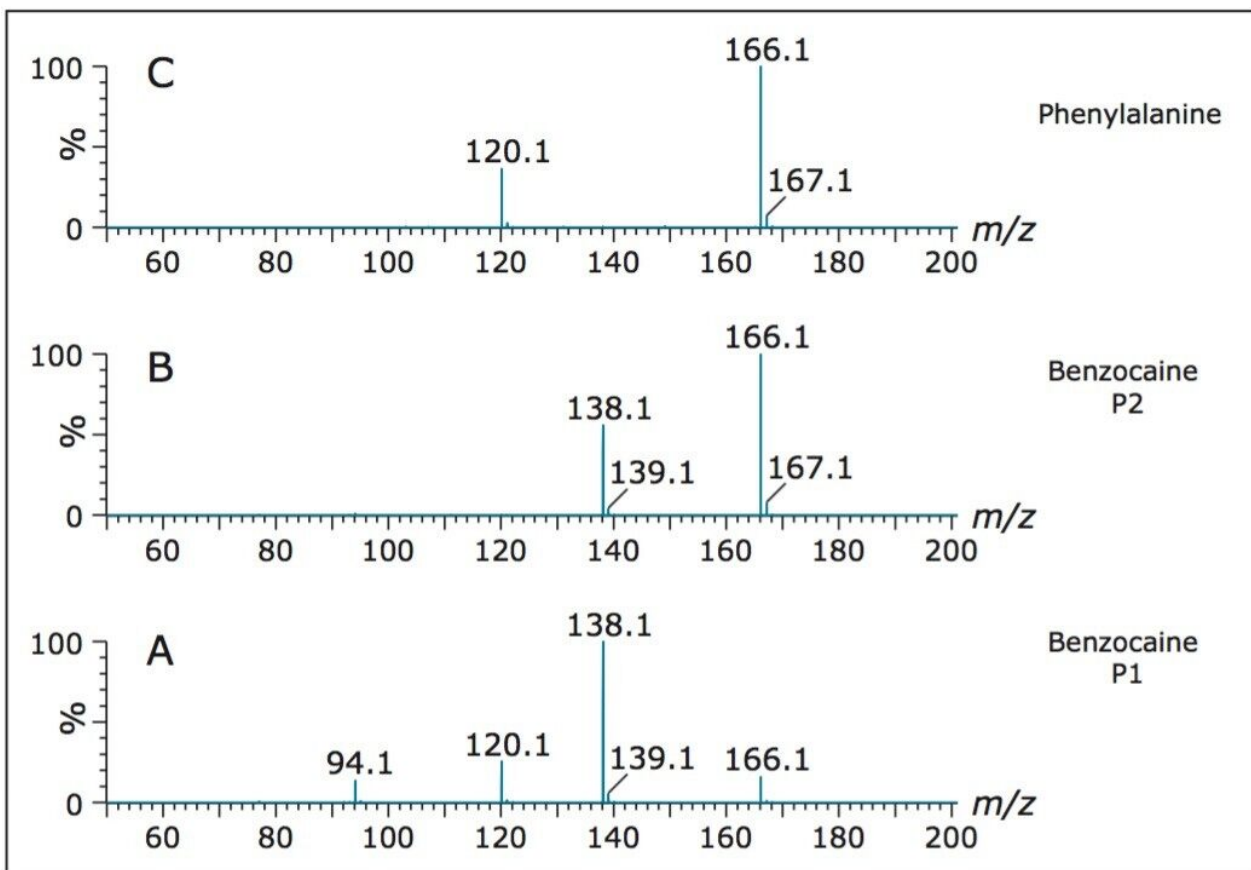


Figure 3. CID product ion mass spectra obtained for the two protonated site isomers of benzocaine: (A) faster drift time, (B) slower drift time, and (C) protonated phenylalanine. The precursor ion at m/z 166 was selected with the quadrupole and induced to fragment within the transfer T-Wave using a collision energy of 15 V following mobility separation in N_2 .

The resulting product ions obtained, and abundances for fragmentation of benzocaine, are due to different fragmentation pathways as a direct result of the different positions of protonation. Both protomers produce a fragment at m/z 138. Both protomers primarily fragment by the neutral loss of C_2H_4 (ethene). The protomer with the fastest drift time shows two other abundant product ions at m/z 120 and m/z 94. Accurate mass measurement confirms these ions to be loss of water from m/z 138 and formation of the the anilinium cation. These product ions suggest protonation on the carbonyl oxygen and not the amide nitrogen

Conclusion

It can be clearly seen that the separation for this simple mixture, although adequate in N₂, is superior in CO₂. This application demonstrates the utility of the ion mobility-MS/MS assay, which is particularly relevant for further multiple reaction monitoring bio-analytical method development in the absence or presence of benzocaine. This will not only have important consequences for the quantitative Phe/Tyr ratio analysis, but the combination of ion mobility to screening protocols will augment other metabolic studies and applications whereby interferences may be present.

References

1. Patricia Hunt. Newborn Screening by Tandem Mass Spectrometry in Texas. 2012.
2. Snelling, JR. Characterisation of pharmaceutical and polymer formulations by novel mass spectrometry approaches. PhD thesis, University of Warwick. 2012.
3. Warnke, S, Seo J, Boschmans J, Sobott F, Scrivens JH, Bleiholder C, Bowers MT, Gewinner S, Schollkopf W, Pagel K, von Helden G. Protomers of Benzocaine: Solvent and Permittivity Dependence. *J Am Chem Soc*. 2015 Mar 17. [Epub ahead of print] .

Featured Products

[SYNAPT G2-Si High Definition Mass Spectrometry <https://www.waters.com/134740622>](https://www.waters.com/134740622)

[Travelling wave \(T-Wave™\) <https://www.waters.com/134663694>](https://www.waters.com/134663694)

720005367, April 2015

©2019 Waters Corporation. All Rights Reserved.