

Note d'application

UPLC-FLR Measurement of Flavanol and Procyanidin Bioactives In Cocoa-Based Commercial Products

Ugo Bussy, Jinchuan Yang, Hong You, Nicholas Anderson, Emily R Britton, Catherine Kwik-Urbe

Mars, Incorporated, Waters Corporation, Eurofins US Food and Nutritional Supplements



Abstract

Recently a hydrophilic interaction liquid chromatography (HILIC)-based method with fluorometric detection was recognized as an Official Method of Analysis for cocoa flavanols and procyanidins with a degree of polymerization 1–7 (AOAC2020.05). This application note demonstrates a successful implementation of AOAC2020.05 on a Waters ACQUITY UPLC H-Class System coupled with the ACQUITY UPLC FLR Detector using a Waters Torus DIOL Column and Waters Oasis PRiME MCX SPE Cartridges. The benefits of thorough system equilibration and sample cleanup are highlighted. This method was successfully applied to commercial cocoa-based foodstuffs and dietary supplements with cocoa flavanol and procyanidin contents ranging from 3–500 mg/g, which demonstrated the versatility and reliability of this routine analysis method for flavanols and procyanidins in these products using Waters equipment and columns.

Benefits

- Waters ACQUITY UPLC H-Class System and ACQUITY UPLC FLR Detector provide an ideal platform for the routine analysis of flavanols and procyanidins in cocoa-based foodstuffs and supplements
- Waters Torus DIOL Column offers excellent and reliable separation of cocoa flavanols and procyanidins
- Waters OASIS PRiME MCX SPE Cartridge effectively removes matrix impurities and ensures reproducible determination of cocoa flavanols and procyanidins

Introduction

Cocoa flavanols and procyanidins (F/PC) are botanical bioactives that have been shown to support healthy blood flow, contributing to cardiovascular and cognition benefits.^{1,2} In cocoa, the flavanols are represented by a possible four monomers ((+/-)-epicatechin and (+/-)-catechin), while procyanidins are oligomers formed from these monomers (Figure 1).³ Given the structural similarities and large number of possible procyanidin structures, they are defined, separated, and measured by degree of polymerization (DP).^{4–6} Because oligomer structure heterogeneity increases exponentially with degree of polymerization, the development of a quantitative, robust, and reliable analytical method has been challenging for the scientific community.

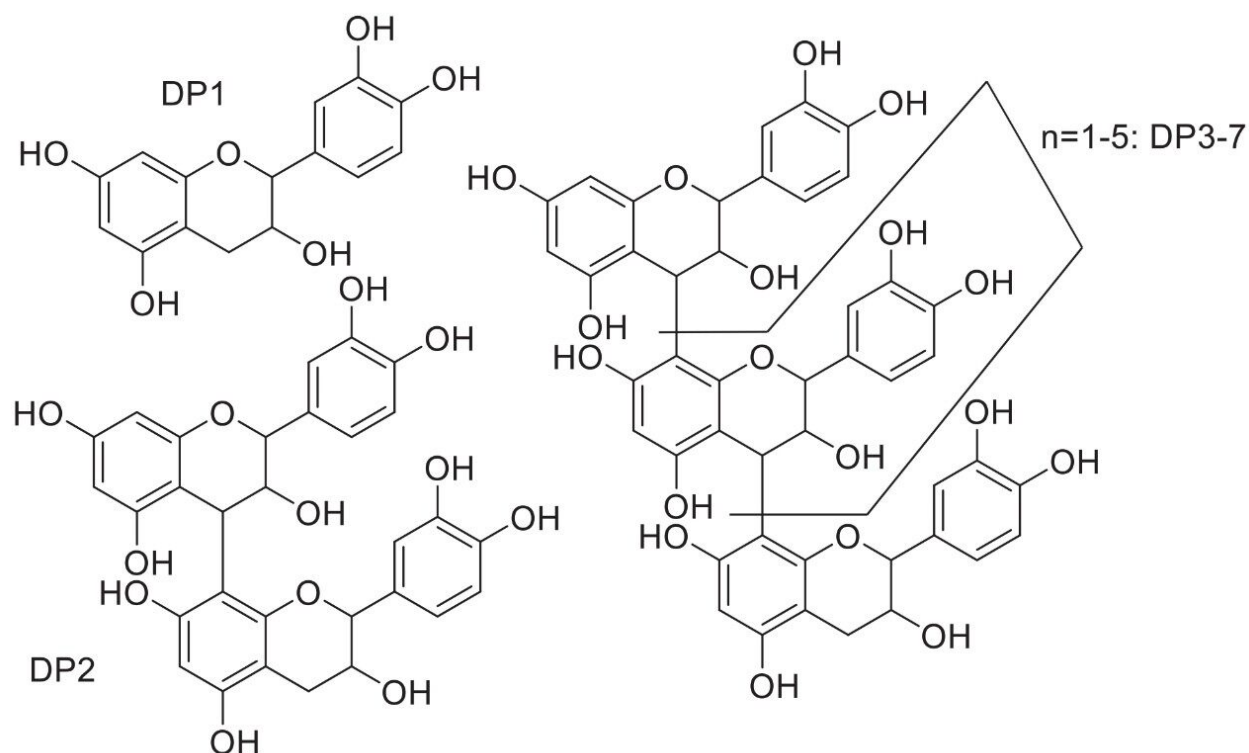


Figure 1. Structures of flavanols (DP1) and procyanidins, including dimer (DP2) and trimer to heptamer (DP3-7).

AOAC International recently recognized a hydrophilic interaction chromatography (HILIC)-based UPLC-FLR method as an official method of analysis for cocoa F/PC, with degree of polymerization 1–7 (Method AOAC2020.05).⁷ This method improves upon a recently published method for the determination of cocoa flavanol and procyanidins by UPLC-FLR⁸ with comprehensive sample preparation for cocoa powder and chocolate matrices.⁹ Because AOAC2020.05 uses HILIC for the separation, system equilibration can be challenging when compared to reverse phase HPLC.¹⁰

In this application note, we describe the implementation of AOAC2020.05 and the impact of system equilibration and sample treatment on the reliability of generated results. This method was applied to 20 cocoa samples to demonstrate applicability to a wide range of concentrations and sample types.

Experimental

Sample Description

Commercially available cocoa-based products, including cocoa powder, baking chocolate, dark chocolate, and cocoa-based dietary supplements (available as a beverage powder and capsules), were purchased from local stores. All samples were identified by their matrix followed by a letter that differentiates various brands/manufacturers; multiple lots of each product were used for this analytical work.

Sample Preparation

All samples were prepared according to AOAC2020.05, except for the dietary supplement capsules. Cocoa powders, dark chocolate, and baking chocolate samples were defatted with consecutive hexane washes. The defatted solid was dissolved and passed through an Oasis PRiME MCX SPE Cartridge to remove matrix impurities. The powdered supplement was suspended in a mixture of acetone, water, and acetic acid (AWA, 70:30:1), sonicated, and centrifuged. Dietary supplement capsules used in this study contained ascorbyl palmitate as an excipient, which causes a significant under-estimation of F/PC and was not removed by SPE treatment. Instead, ascorbyl palmitate was removed by solid-liquid extraction with two consecutive washes using hexane:isopropanol 100:5 (v/v).

Standard Preparation

Calibration standards were prepared as described in AOAC2020.05, with a serial dilution of NIST cocoa flavanol extract reference material RM8403.¹¹ Briefly, 20 mg of RM8403 were weighed in a 100-mL volumetric flask and dissolved with AWA to prepare working standard 5 (WS5). WS1–4 were prepared by pipetting 2, 4, 6, and 8 mL of WS5 in 10-mL flasks and diluting with AWA.

Method Conditions

LC Conditions

LC system:	ACQUITY UPLC
	H-Class
Detection:	ACQUITY UPLC
	FLR Detector;
	gain 10, emission
	321 nm and excitation 230 nm

LC Conditions

Note: gain must
be optimized for
each instrument
on which
AOAC2020.05 is
implemented

Vials/Plates:

LCMS Certified
Amber Glass 12 x
32 mm Screw
Neck Vial, with
Cap and Preslit
PTFE/Silicone
Septum, 2 mL
(p/n:
600000669CV)

Column(s):

Torus DIOL, 130Å,
1.7 µm, 3.0 mm x
100 mm

Column temp.:

50 °C

Sample temp.:

5 °C

Injection volume:

2 µL

Flow rate:

1.00 mL/min

Mobile phase A:

Acetonitrile:acetic
acid 98:2 (HPLC-
grade)

LC Conditions

Mobile phase B: Methanol:water:acetic
acid 95:3:2
(HPLC-grade)

Data management: Empower 3 CDS

Gradient

Time (min)	Flow (mL/min)	%A	%B	Curve
0.00	1.00	100	0	6
0.37	1.00	100	0	6
10.40	1.00	55	45	6
10.65	1.00	5	95	6
13.00	1.00	5	95	6
13.10	1.00	100	0	6
16.10	1.00	100	0	6


Sequence of injection

1. Five injections of cocoa extract reference material – for system equilibration
2. Five injections of cocoa extract reference material – for system suitability (repeatability)
3. Calibration curve injections
4. Blank
5. Sample injections (up to 10)
6. Cocoa extract reference material injection – system suitability (bracketing)

Results and Discussion

Using the ACQUITY UPLC H-Class System coupled with FLR detection, cocoa F/PC with a DP up to seven were separated and analyzed in 16 minutes, as shown in Figure 2. Cocoa F/PC were chromatographically separated using a Waters Torus DIOL Column by degree of polymerization and integrated as seven independent signals, from monomer (DP1) to heptamer (DP7).

After inadequate conditioning: Injections 1, 5, and 10

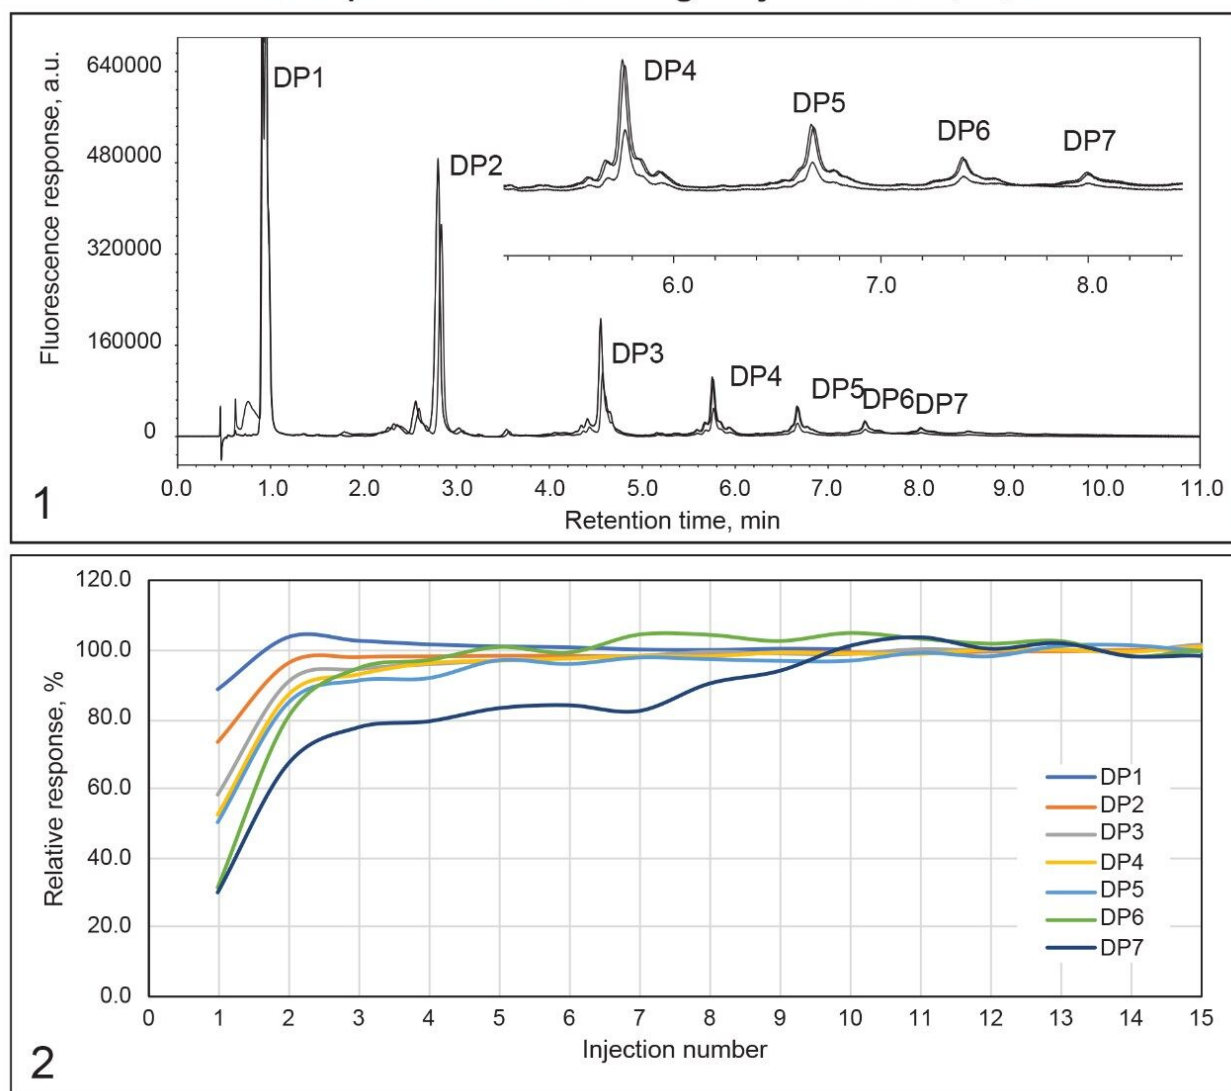

After adequate conditioning: Injections 1, 5, and 10

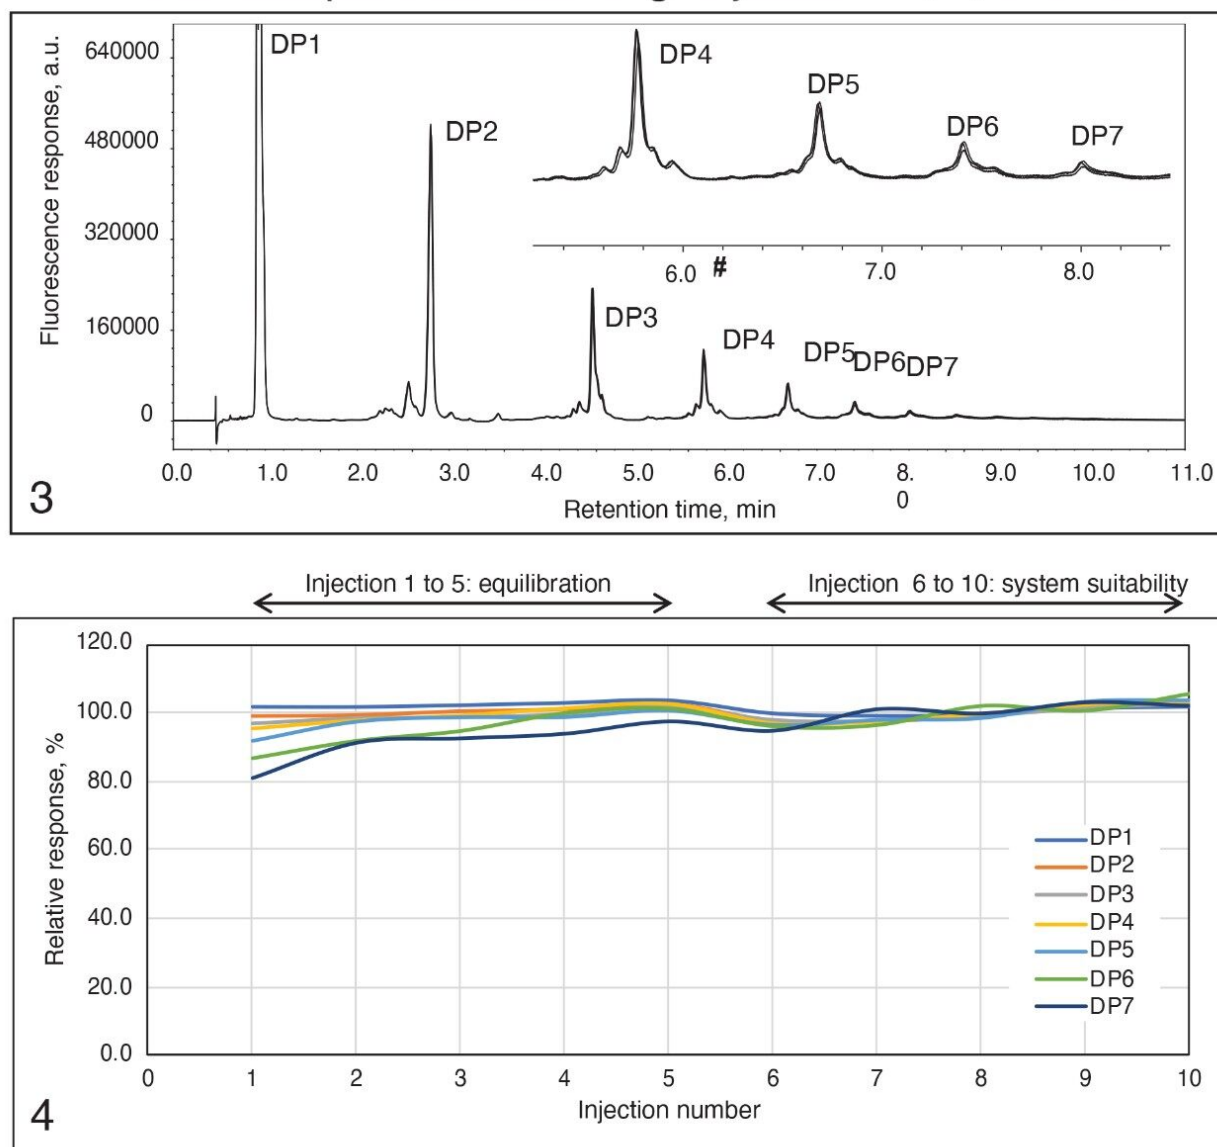


Figure 2. Effect of method equilibration on repeatability of DP1-7 signals. Panels 1 and 3: overlay of first, fifth, and 10th repeated injection of NIST RM8403; Panels 2 and 4: relative response for 15 and 10 repeated injections of NIST RM8403, respectively.

System Equilibration

The separation of cocoa F/PC is achieved under HILIC conditions and requires the equilibration of the system prescribed by AOAC2020.05. Detector response requires equilibration (system purge, column wash, and conditioning sample injections) to reach repeatable output, although reproducible retention of neutral

polar targets could be rapidly achieved under HILIC conditions.¹² In this context, the thorough integration of signals is essential to achieving precise measurement. For F/PC, a multitude of stereoisomers contributed to each signal, leading to wide peak shape and the need for a valley-to-valley integration. This valley-to-valley integration could be strongly impacted by poorly equilibrated systems often showing fluctuating baseline. Figure 2 showed the relative signal area for each of the seven targeted signals with inadequate and adequate equilibration. Relative signal responses were calculated as the ratio of signal area in the injection to the average signal area of the final five injections of the sequence. In an equilibrated system, relative responses were expected to plateau around 100%.

Adequate equilibration is achieved following the protocol defined by AOAC2020.05:

- Purge each solvent line for 5 min at 4 mL/min before mounting column
- Equilibrate the column for at least 10 min with 50:50 mobile phase A/B
- Finalize system equilibration by running at initial conditions (1 mL/min at 100% A) for approximately 10 min
- Complete equilibration with 10 injections of cocoa extract reference material

Inadequate equilibration procedure, such as 1 min of solvent purge, 5 min of column equilibration, and 5 min of system equilibration followed by multiple injections of cocoa extract reference material was conducted to demonstrate the necessity of adequate equilibration.

As shown by Figure 2, adequate equilibration of the system leads to precise measurement of signal area between injections, while inadequate equilibration significantly impacts the response of the target signal. In addition to significantly impacting the assessment of repeatability criteria of the system suitability, inaccurate estimation of the response during repeatability injection can challenge the reliability of the following injections. The average signal area of the last five repeatability injections is used to evaluate the response of bracketing standard injections. The evaluation of bracketed standard response was a critical requirement of system suitability as it allows for the verification that adequate system performance for sample analysis is maintained throughout the sequence.

Sample Cleanup

To evaluate the impact of sample cleanup on method reliability and subsequent data quality, system performances were compared after 10 injections of baking chocolate prepared in three different ways: no SPE, strong cation exchange SPE, and mixed-mode polymeric SPE with cation exchange groups (Waters Oasis PRiME MCX). The signal area of a bracketing standards injection, following the injections (n=10) of baking chocolate was compared to the initial repeatability system suitability injection and % recoveries were

calculated.

The % recoveries for each DP measured in the bracketing standard are used as a marker of the effect of injecting samples on system performances and are shown in Table 1. All procyanidin signals (DP2–7) were significantly impacted after 10 injections of the sample that did not undergo SPE treatment alongside an increase in system back pressure. Signal area was observed to be 25% higher than the expected value and associated with interferences, leading to a failure to meet system suitability and demonstrating the importance of properly removing co-eluting matrix impurities that interfere with the analysis. System performance was recovered after a wash with water:isopropanol (50:50), which allowed the elution of column contaminants, resulting in a decrease of back pressure. The system was then put through the full equilibration process. The cleanup of baking chocolate samples using the strong cation exchange SPE cartridge led to a slight improvement in recoveries. However, there was still a significant impact of samples on system back pressure (50–100 bar build up) and a clear drift in signal responses for higher order oligomers (DP3–7).

Analyte		DP1	DP2	DP3	DP4	DP5	DP6	DP7
Repeatability (%RSD; n=5)		1	2	2	3	3	4	3
Bracketing standard recovery (%)	AOAC2020.05 acceptance criteria	95–105	95–105	95–105	95–105	90–110	80–120	80–120
	No SPE	100	106*	110*	110*	112*	116	125*
	Strong cation exchange SPE	102	103	108*	110*	111*	114	121*
	MCX PRiME	100	104	103	102	101	103	101

Table 1. Relative recovery of bracketing standard injections after ten injections of a baking chocolate sample prepared without SPE cleanup, strong cation exchange SPE cleanup, and mixed mode cation exchange SPE clean up.

**Denote bracketing standard recovery failure to meet system suitability criteria as defined by AOAC2020.05.*

Sample treatment using Oasis PRiME MCX SPE cartridges contributed to precise and accurate determination of cocoa F/PC. As shown in Table 1, there was little deviation of % standard recovery when mixed mode SPE cleanup was implemented. Repeatability was calculated as the relative standard deviation for injection 6–10 of the system suitability. Recovery is determined relatively to the average peak area observed in injection 6–10 of the system suitability section. The adequate cleanup is associated to the sorbents capacity to retain more matrix co-extractives through the mixed mode retention mechanisms (reversed-phase and cation exchange). In addition, the mixed mode SPE also support the removal of charged

lipids or excipients (such as magnesium stearate) providing a sample free from impurities that would contaminate the system, generate increased back pressures and interfere with fluorescence detection. Successful cleanup of samples was demonstrated by observing a stable system pressure and reproducible bracketing standard injections.

For certain matrices (e.g., dietary supplements formulated at higher concentration), SPE cleanup of the sample was not necessary. In fact, highly concentrated samples such as dietary supplements were less subject to matrix interferences during the analysis. Sample preparation can be optimized for a specific matrix after not only demonstrating key performances such as accuracy and precision but showing no impact on system performances beyond the sample analyzed.

Application to Commercially Available Samples

Method performance has been previously demonstrated and published.⁹ However, limited data had been published on the application of AOAC2020.05 methodology to the determination of real samples. Twenty cocoa-based commercially available products were purchased and analyzed per AOAC2020.05. Table 2 summarizes the contents determined for cocoa flavanols (DP1) and individual oligomers (DP2–7) as well as the total cocoa F/PC for commercially available products including dark and baking chocolates, cocoa powders, ready-to-mix dietary supplement powder, and dietary supplement capsules (alphabetical suffixes indicate different brands, numerical suffixes indicate different lots). Samples were determined to contain total cocoa flavanol and procyanidin contents ranging from 2.9 to 524 mg/g, demonstrating that a wide range of cocoa-based products can be characterized using AOAC2020.05. In addition, identical products (same brand and products, different lot number) showed comparable results. This suggests that the high precision achieved on the measurement of cocoa F/PC can support the discrimination of samples by matrix type and manufacturing origins as previously reported.⁸

Matrix	DP1 (mg/g)	DP2 (mg/g)	DP3 (mg/g)	DP4 (mg/g)	DP5 (mg/g)	DP6 (mg/g)	DP7 (mg/g)	Total DP1-7 (mg/g)
Dark chocolate A1	1.1	0.8	0.8	0.6	0.6	0.4	0.2	4.6
Dark chocolate A2	1.0	0.8	0.8	0.6	0.5	0.4	0.3	4.3
Dark chocolate B	0.6	0.5	0.5	0.4	0.5	0.4	0.1	3.0
Baking chocolate A1	1.0	1.0	0.9	0.7	0.5	0.4	0.1	4.7
Baking chocolate A2	0.9	0.8	0.8	0.6	0.5	0.4	0.1	4.1
Baking chocolate A3	0.6	0.5	0.5	0.4	0.4	0.3	0.2	2.9
Baking chocolate B1	1.1	1.3	1.4	1.2	1.0	0.8	0.7	7.4
Baking chocolate B2	1.1	1.3	1.4	1.1	1.0	0.8	0.6	7.3
Cocoa powder A1	3.3	2.5	2.2	1.6	1.3	1.0	0.4	12.3
Cocoa powder A2	3.3	2.6	2.3	1.6	1.3	1.0	0.5	12.6
Cocoa powder A3	3.0	2.5	2.3	1.8	1.5	1.1	0.5	12.6
Cocoa powder B	3.4	3.1	3.1	2.6	2.2	1.6	0.7	16.7
Cocoa powder C	4.2	3.8	3.6	2.8	2.4	1.6	0.8	19.3
Ready-to-drink supplement A1	13.6	12.6	15.6	12.2	10.3	8.4	6.0	78.6
Ready-to-drink supplement A2	12.2	11.5	13.7	11.8	9.7	7.6	5.4	71.8
Ready-to-drink supplement B1	17.8	12.9	13.7	12.1	10.0	7.8	6.1	80.4
Ready-to-drink supplement B2	19.3	14.1	15.0	12.2	10.9	8.4	6.4	86.4
Supplement capsule A1	116.1	81.2	86.6	74.5	66.0	52.4	40.5	517.5
Supplement capsule A2	116.4	81.0	86.7	76.7	67.0	51.6	45.2	524.5
Supplement capsule B	109.4	78.8	85.1	73.5	63.4	50.8	41.4	502.3

Table 2. Summary of cocoa flavanol and procyanidin content in cocoa-based commercial products.

Conclusion

The Official Method of Analysis AOAC2020.05 was implemented for the analysis of cocoa flavanols and procyanidins with degree of polymerization of up to seven in cocoa-based matrices. The impact of method equilibration was estimated using the required method system suitability criteria. The equilibration steps outlined in this application note, while lengthy, have been shown to be critical for method performance and should be implemented with each batch of sample analysis. When equilibrating the system as prescribed in AOAC2020.05, precise and consistent results are achieved and demonstrated through system suitability.

System suitability was used to monitor system performances and estimate the bias introduced by inadequate sample preparation using the example of baking chocolate. In addition to increasing system back pressure, the contamination of the system with matrix impurities led to an overestimation of procyanidin content by up to 25%. These interferences were remediated through sample processing using mixed mode cation exchange and charged lipid removal solid phase extraction.

Finally, the method was successfully applied to the determination of commercial cocoa-based foodstuffs and dietary supplements with cocoa flavanol and procyanidin contents ranging from 3 to 500 mg/g. These results together with system suitability experiments demonstrated the versatility of the AOAC2020.05 methodology and its reliability for the routine analysis of flavanols and procyanidins in cocoa-based foodstuffs and supplements.

References

1. Brickman AM, Khan UA, Provenzano FA, Yeung LK, Suzuki W, Schroeter H, Wall M, Sloan RP, Small SA. Enhancing Dentate Gyrus Function with Dietary Flavanols Improves Cognition in Older Adults. *Nat. Neurosci.*, 2014, 17(12): 1798–803.
2. Heiss C, Sansone R, Karimi H, Krabbe M, Schuler D, Rodriguez-Mateos A, Kraemer T, Cortese-Krott MM, Kuhnle GG, Spencer JP, Schroeter H, Merx MW, Kelm M, Flaviola Consortium, E.U.t.F.P. Impact of Cocoa Flavanol Intake On Age-Dependent Vascular Stiffness In Healthy Men: A Randomized, Controlled, Double-Masked Trial. *Age (Dordr)*, 2015, 37(3): 9794.
3. Kelm MA, Johnson JC, Robbins RJ, Hammerstone JF, Schmitz HH. High-Performance Liquid Chromatography Separation and Purification of Cacao (*Theobroma cacao* L.) Procyanidins According to Degree of Polymerization Using a Diol Stationary Phase. *J. Agric. Food Chem.*, 2006, 54(5): 1571–6.
4. Adamson GE, Lazarus SA, Mitchell AE, Prior RL, Cao G, Jacobs PH, Kremers BG, Hammerstone JF, Rucker RB, Ritter KA, Schmitz HH. HPLC Method for The Quantification of Procyanidins in Cocoa and Chocolate Samples and Correlation to Total Antioxidant Capacity. *J. Agric. Food Chem.*, 1999, 47(10): 4184–4188.
5. Hammerstone JF, Lazarus SA, Mitchell AE, Rucker R, Schmitz HH. Identification of Procyanidins in Cocoa (*Theobroma cacao*) and Chocolate Using High-Performance Liquid Chromatography/Mass Spectrometry. *J. Agric. Food Chem.*, 1999, 47(2): 490–496.
6. Lazarus SA, Adamson GE, Hammerstone JF, Schmitz HH. High-Performance Liquid Chromatography/Mass Spectrometry Analysis of Proanthocyanidins in Foods and Beverages. *J. Agric. Food Chem.*, 1999, 47(9): 3693–701.
7. AOAC. 2020: Official Method of Analysis 2020.05.
8. Bussy U, May BR, Olanrewaju Y, Hewitt G, Anderson N, Crozier A, Ottaviani JI, Kwik-Urbe C. Reliable,

Accessible, and Transferable Method for the Quantification of Flavanols and Procyanidins in Foodstuffs and Dietary Supplements. *Food Funct.*, 2020, 11(1): 131–138.

9. Bussy U, Hewitt G, Olanrewaju Y, May BR, Anderson N, Ottaviani J, Kwik-Urbe C. Single-Laboratory Validation for the Determination of Cocoa Flavanols and Procyanidins (by Degree of Polymerization DP1–7) in Cocoa-Based Products by Hydrophilic Interaction Chromatography Coupled with Fluorescence Detection: First Action 2020.05. *J. AOAC Int.*, 2020.
10. McCalley DV. A Study of Column Equilibration Time in Hydrophilic Interaction Chromatography. *J. Chromatogr. A*, 2018, 1554: 61–70.
11. Rimmer CA, Lippa KA, Yen J, Bussy U, Anderson N, Kwik-Urbe C. Reference Material 8403 Cocoa Flavanol Extract. *NIST Special Publication*, 2020.
12. Bell DS, Shollenberger DL. Investigation of Reequilibration in Hydrophilic Interaction Liquid Chromatography. *LCGC*, 2016 29(12): 687–692.

Acknowledgements

Ugo Bussy (Mars, Incorporated), Jinchuan Yang (Waters Corporation), Hong You (Eurofins US Food and Nutritional Supplements), Nicholas Anderson (Mars, Incorporated), Emily R Britton (Waters Corporation), and Catherine Kwik-Urbe (Mars, Incorporated).

Featured Products

ACQUITY UPLC H-Class PLUS System <<https://www.waters.com/10138533>>

ACQUITY UPLC FLR Detector <<https://www.waters.com/514222>>

Empower Chromatography Data System <<https://www.waters.com/waters/nav.htm?cid=513188>>

720007121, January 2021

