

응용 자료

Extraction and Analysis of a Definitive Drug Panel in Hair Samples by UHPLC-MS/MS for Forensic Toxicology

Jonathan Danaceau, Lisa Calton

Waters Corporation, United States

Published on June 10, 2025

Contact Sales

For forensic toxicology use only.

Abstract

This application note describes a robust UHPLC-MS/MS method for the analysis of drugs of abuse in hair to satisfy the confirmation cut-off values as recommended by the Society of Hair Testing (SoHT).^{1,2} Many common forensically relevant drugs are included including opiates, amine stimulants, benzodiazepines, fentanyl and other synthetic opiates, and other common drugs of abuse. Extraction conditions were optimized to address the wide variety of compounds. The samples were then cleaned up using Oasis™ MCX mixed-mode cation exchange plates and separated on an ACQUITY™ UPLC™ I-Class Plus System. The Xevo™ TQ Absolute Triple Quadrupole Mass Spectrometer provided the specificity and sensitivity to meet the detection requirements outlined by the SoHT.

Benefits

- Hair matrix provides long drug detection window and collection is non-invasive
- Optimized sample preparation for a wide variety of compounds
- Robust method using UHPLC-MS/MS for the sensitive determination of forensically relevant drugs in hair

Introduction

The use of hair as a biological matrix for forensic testing continues to increase in popularity. As a specimen, hair offers several benefits. In contrast to other matrices such as blood, hair collection is simple and does not require medically trained staff to collect the sample. Sample collection is not considered intrusive, meaning that collection can be easily supervised, thus reducing the potential for sample adulteration. Further, once collected, hair can be easily transported and stored at room temperature prior to analysis.

Drug substances can be incorporated into the hair by various mechanisms including passive diffusion from the blood supply at the follicle into the growing hair matrix, diffusion into the hair shaft from sweat or sebum or external contamination such as smoke or contaminated hands. Some key factors that affect the incorporation of hair include the melanin content of the hair, pKa of the analyte and the degree of lipophilicity of the analyte.

One key benefit of hair is that it provides an extended window of detection for drug exposure. Unlike traditional matrices such as blood and urine, where drugs may only be detected within hours or days of use, drugs can be detected in hair months and even years after use. Hair generally grows at a rate of 1 cm per month. Thus, a hair sample can provide an accumulated specimen which can provide an insight into drug usage over recent months. This makes analysis of illicit drugs and pharmaceuticals in hair useful for situations where other samples may not be appropriate or available for analysis such as post-mortem toxicology, drug facilitated sexual assault (DFSE), or for employment testing in which long-term monitoring is desired.

Hair analysis does have some challenges that must be addressed, however. First, hair must be decontaminated prior to analysis to remove surface contamination. The pulverization step is also critical. More complete pulverization leads to more efficient extraction for many common drugs (Hu 2023, JAT; 47; 346–52).³ The initial extraction conditions are also crucial. Some drugs and metabolites are unstable at either high or low pH, and solvent composition can affect the efficiency of the extraction for different compounds. All these issues must be

considered and balanced when extracting a large panel of compounds from hair.

In developing this analytical method, we were able to optimize the initial incubation to efficiently extract a wide variety of compounds including opiates, amine stimulants, benzodiazepines, synthetic opiates, and other forensically relevant compounds while meeting the sensitivity requirements of the Society of Hair Testing (SoHT). Oasis MCX plates enabled a quick and efficient sample clean up. Analyte recoveries were consistent and resulted in the accuracy and precision needed for this assay. Rapid separation was achieved with the ACQUITY UPLC I-Class Plus System and ACQUITY BEH™ Column coupled to the Xevo TQ Absolute Triple Quadrupole Mass Spectrometer which provided the sensitivity required for this analysis.

Experimental

LC/MS grade solvents were either from Fisher or Honeywell. Optima Grade formic acid and ammonium acetate were from Fisher Scientific. Certified reference materials and internal standards were acquired from Cerilliant (Round Rock, TX).

Hair samples were sourced from volunteers and analyzed as either single samples or blended.

External positive control samples were purchased from Comedical (Comedical.biz).

Certified reference standards and mixes were combined to make a nominal 10 µg/mL working stock solution which was then further diluted to produce working calibrator and quality control standards. 6-acetyl morphine and norfentanyl had a concentration of 2 µg/mL and fentanyl had a concentration of 1 µg/mL in the working stock solution. Seven working standards were prepared, ranging from 10–1000 ng/mL in methanol (MeOH). Quality control working stock solutions were prepared at concentrations of 30, 150, and 300 ng/mL in methanol. An internal standard (IS) stock solution was prepared at 1000 ng/mL in methanol. Working IS solutions were prepared daily in methanol at 250 ng/mL.

A volume of 20 µL of each working calibrator or control standard was added to 20 mg of hair, resulting in a nominal calibration range from 0.01–1.0 ng/mg and QC samples at concentrations of 0.03, 0.15, and 0.30 ng/mg hair.

Extraction Method

Hair samples were decontaminated by sequential solvent washes and allowed to fully dry. Bulk hair samples were pulverized using a Precellys Tissue Homogenizer and 2 mL CKMix Lysing Kits (Bertin Technologies, Montigny-le-Bretonneux, FR) for 6 x 6400 rpm for 40 seconds each.

An aliquot of blank, pulverized hair (20 ± 1 mg) was weighed into 16 x 100 mm round bottomed glass centrifuge tubes. Working calibrator and QC solutions were added as described above along with 40 μ L of working IS solution. A double blank sample was also prepared with no IS. Next, 1.2 mL of the extraction solution was added and then the tubes were capped, and samples were incubated for 2 hrs at 95 °C. The samples were then centrifuged at 3200 rcf for 5 min and the solvent was transferred to a 2 mL 96-well collection plate containing 25 μ L of formic acid. Sample extracts were evaporated for approximately 30 minutes to remove most of the solvent. After evaporation, samples were diluted with 1.5 mL of 4% phosphoric acid and loaded onto the wells of a Waters MCX 96-well plate (30 mg/well; p/n 186000258). The wells were then washed with 2 x 1 mL 80:20 water:methanol and eluted with 2 x 125 μ L of 50:50 ACN:MeOH containing 5% strong ammonia (28–30%) and diluted with 500 μ L of 97:2:1 water:ACN:formic acid. The entire extraction workflow is shown in Figure 1.

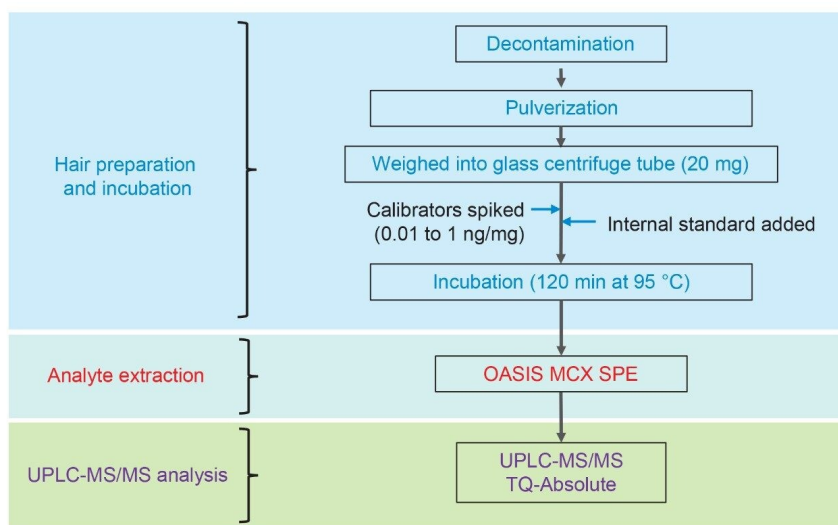


Figure 1. Workflow used for the extraction of drugs from Hair.

Chromatographic separation was achieved using a gradient of water and acetonitrile, both containing 0.1% formic acid, on an ACQUITY UPLC BEH C₁₈ Column, 1.7 μ m, 2.1 x 100 mm. The UHPLC System conditions are displayed below.

LC Conditions

LC system:	ACQUITY UPLC I-Class PLUS System
Column:	ACQUITY UPLC BEH C ₁₈ 1.7 µm, 2.1 x 100 mm
Column temperature:	40 °C
Sample temperature:	10 °C
Injection volume:	2 µL
Flow rate:	0.6 mL/min
Mobile phase A:	0.1% formic acid in MilliQ water
Mobile phase B:	0.1% formic acid in acetonitrile
Wash solvent:	25:25:25:25 MeOH:H ₂ O:IPA:ACN

Gradient Table

Time (min)	Flow (mL/min)	%A	%B	Curve
0	0.6	98	2	6
3.33	0.6	33	67	6
3.5	0.6	10	90	6
3.6	0.6	98	2	6
4	0.6	98	2	6

MS Conditions

MS system:	Xevo TQ Absolute Triple Quadrupole Mass Spectrometer
Ionization mode:	ESI positive
Desolvation temperature:	500 °C
Desolvation gas flow:	1000 L/hr
Cone gas flow:	150 L/hr
Acquisition range:	MRM transitions optimized for individual compounds
Capillary voltage:	1.0 kV
Collision energy:	Optimized for individual compounds (See Appendix 1)
Cone voltage:	Optimized for individual compounds (See Appendix 1)

Data Mangement

MS software:	MassLynx™ Mass Spectrometry Software
Quantification software:	TargetLynx™ XS / QUAN Review

Results and Discussion

Figure 2 shows the resulting chromatography using the UPLC BEH C₁₈ Column. Individual retention times are

listed in Appendix 1. These chromatographic conditions were the same as those used previously for a multi-analyte panel in urine (Danaceau, 2017; [720006187 <https://www.waters.com/nextgen/global/library/application-notes/2019/comprehensive-method-for-the-analysis-of-pain-management-drugs-and-drugs-of-abuse.html>](https://www.waters.com/nextgen/global/library/application-notes/2019/comprehensive-method-for-the-analysis-of-pain-management-drugs-and-drugs-of-abuse.html)). All compounds were baseline separated from any potentially interfering compounds and internal standards as shown previously. All compounds were eluted by 3.2 minutes with a total LC cycle time of 4.0 minutes.

The sample preparation procedure was rapid, clean and robust. Figure 3 shows the recovery and matrix effects for all the compounds. Recoveries averaged 58% with 49/58 >40%. Some compounds such as the amine stimulants and EDDP demonstrated lower than average recovery. However, it was consistent and enabled the accurate and precise quantification of all compounds even at the lowest concentration levels. Matrix effects averaged 20% with only 6 compounds exceeding 40% ion suppression. The use of deuterated internal standards corrected for this, allowing accurate analyte quantification. As shown in Figure 3, matrix effects were consistent, with standard deviations all under 10%.

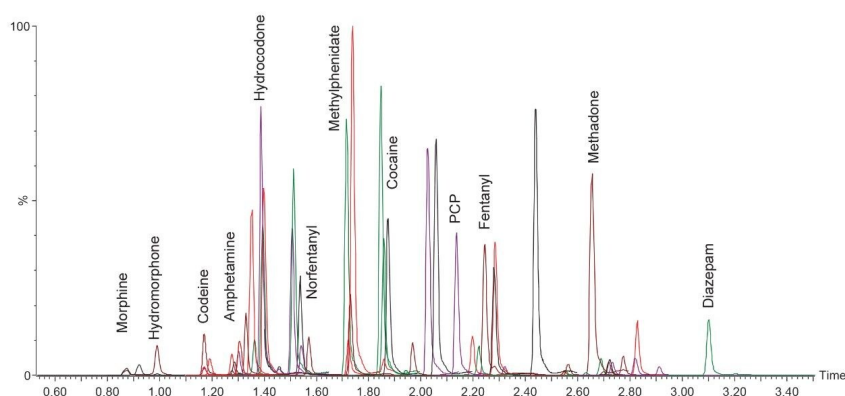


Figure 2. Chromatography of the forensic toxicology panel extracted from hair samples. The column was a Waters BEH C₁₈ 1.7 μ m, 2.1 x 100 mm Column. Several key compounds are labelled.

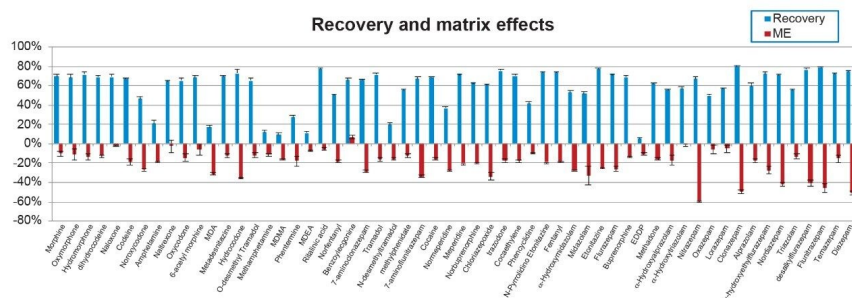


Figure 3. Recoveries and matrix effects from the incubation and solid phase extraction procedure. Recoveries averaged 58% with 49/58 >40% and matrix effects averaged 20% with only 6 compounds exceeding 40% ion suppression. All %RSDs were <10% for the recovery data and standard deviations were <10% for the matrix effects data.

Several factors proved to be critical when optimizing the sample preparation procedure. For example, optimizing the incubation solution significantly improved recoveries for oxazepam and lorazepam. Additionally, the use of formic acid vs. HCl during in the evaporation step was necessary to prevent the acid catalyzed degradation of alprazolam, triazolam, and midazolam. Enzymatic digestion was also initially investigated as a sample pretreatment method. However, it needed an overnight digestion, many compounds demonstrated substantial ion suppression (>80%), and we saw significant chromatographic interferences, so it was not investigated further.

Calibration curves ranged from 0.01–1.0 ng/mg, encompassing the cutoff values of the Society of Hair Testing for drugs of abuse. As mentioned above, 6-acetyl morphine (6-AM) and norfentanyl had calibration ranges from 0.002–0.2 ng/mg and fentanyl had a calibration range from 0.001–0.1 ng/mg. All compounds had R^2 values of 0.99 or better, apart from phentermine and metadesnitazine. Neither of these compounds had a stable labelled internal standard and phentermine was also subject to significant matrix-based interference. Figure 4 shows calibration curves for morphine, methamphetamine, fentanyl, and alprazolam.

Accuracy and precision were evaluated by extraction of 5 individual batches. The results are shown in Appendices 2 and 3. All compounds had within-run and between-run accuracies within 15% of target values (20% for low QC samples) and %CVs <15% (20% for the low QC samples), apart from phentermine and metadesnitazine. The remainder of the compounds demonstrated accuracy and precision values that met the

validation requirements of ASB Standard-036.

Functional sensitivity was assessed by extracting 10 replicates at nominal concentrations of 0.01 and 0.02 ng/mg. Lower limits of quantification (LLOQ) were those at which accuracy was within 20% and %CVs were also less than 20%. The results of these experiments are shown in Table 1. For those analytes that did not meet the requirements at 0.01 or 0.02 ng/mg, the low QC was used as a LLOQ. This included MDA, α -OH midazolam and clonazepam. All compounds met the SoHT requirements for sensitivity except for phentermine, which lacked a labelled internal standard and was subject to endogenous interferences. LLOQ values for fentanyl, 6-AM and norfentanyl were correspondingly lower due to their lower calibration ranges.

True accuracy was assessed using external positive control samples from Comedical. These samples had known concentrations of drugs incorporated into the hair matrix as well as established acceptance windows. The results are shown in Table 2. Coefficients of variance were excellent, with all under 10%. Of the compounds included, 18/24 (75%) were within the acceptance criteria established by the manufacturer. The values in the EQA samples were beyond the calibration range of 6-AM and fentanyl, which had upper quantitation limits of 0.2 and 0.1 ng/mg, respectively. Excluding those two, 18/22 (82%) of the compounds met the acceptance criteria. These samples had been prepared by spiking bulk hair with analytes followed by extensive mixing, versus actual hair samples with incorporated drugs. Nevertheless, the comparison is quite favorable.

4a

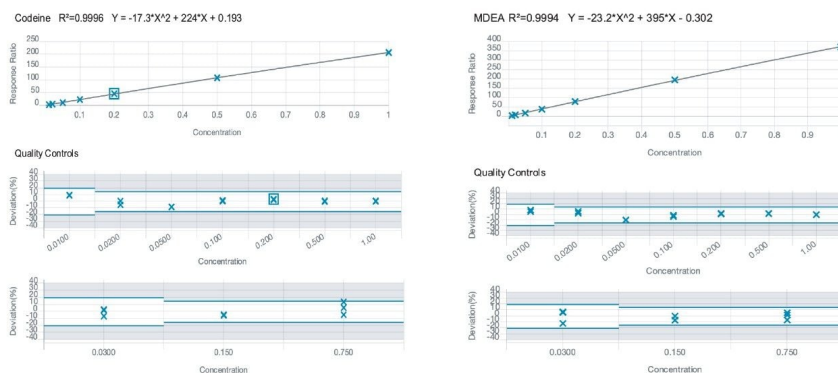


Figure 4a. Calibration curves and quality control results for codeine and MDEA generated by Waters Quan Review software. The upper panels show the calibration curves and the lower panels show the percent deviations and acceptable values for the calibration points and the quality control (QC) samples.

4b

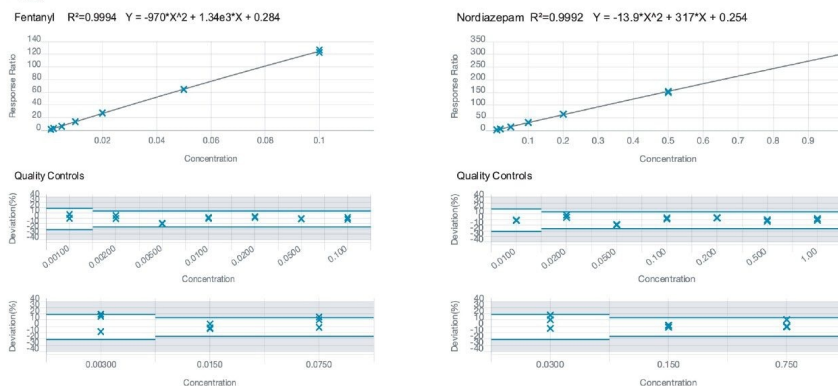


Figure 4b. Calibration curves and quality control results for fentanyl and nordiazepam generated by Waters Quan Review software. The upper panels show the calibration curves and the lower panels show the percent deviations and acceptable values for the calibration points and the quality control (QC) samples.

	LLOQ			LLOQ	
	LLOQ	SoHT Cut-off		LLOQ	SoHT Cut-off
Morphine	0.01	0.20	Meperidine	0.01	0.20
Oxymorphone	0.01	0.20	Norbuprenorphine	0.01	0.01
Hydromorphone	0.01	0.20	Chloriazepoxide	0.01	0.05
Dihydrocodeine	0.01	0.20	Trazodone	0.01	0.20
Naloxone	0.01	0.20	Cocaethylene	0.01	0.05
Codeine	0.01	0.20	Phencyclidine	0.01	—
Noroxycodone	0.01	0.20	N-Pyrrolidino Etonitazine	0.01	—
Amphetamine	0.01	0.20	Fentanyl	0.001	0.20
Naltrexone	0.01	0.20	α -Hydroxymidazolam	0.03	0.05
Oxycodone	0.01	0.20	Midazolam	0.01	0.05
6-acetyl morphine	0.002	0.20	Etonitazine	0.01	—
MDA	0.03	0.20	Flurazepam	0.01	0.05
Metadesnitazine	—	n/a	Buprenorphine	0.01	0.01
Hydrocodone	0.01	0.20	EDDP	0.01	0.05
O-desmethyl Tramadol	0.01	0.20	Methadone	0.01	0.20
Methamphetamine	0.01	0.20	α -Hydroxyalprazolam	0.01	0.05
MDMA	0.01	0.20	α -Hydroxytriazolam	0.01	0.05
Phentermine	—	0.20	Nitrazepam	0.01	0.05
MDEA	0.01	0.20	Oxazepam	0.02	0.05
Ritalinic acid	0.01	n/a	Lorazepam	0.02	0.05
Norfentanyl	0.002	0.20	Clonazepam	0.03	0.05
Benzoyllecgonine	0.01	0.05	Alprazolam	0.01	0.05
7-aminoclonazepam	0.01	0.05	2-hydroxyethylflurazepam	0.01	0.05
Tramadol	0.01	0.20	Nordiazepam	0.01	0.05
N-desmethyltramadol	0.01	0.20	Triazolam	0.01	0.05
Methylphenidate	0.01	—	Desalkylflurazepam	0.01	0.05
7-aminoflunitrazepam	0.01	0.05	Flunitrazepam	0.01	0.05
Cocaine	0.01	0.50	Temazepam	0.01	0.05
Normeperidine	0.01	0.01	Diazepam	0.01	0.05

Table 1. Lower limits of quantification (LLOQ) Limits of quantification for each compound. Established LLOQs and SoHT cutoffs are listed for each compound. For those without cutoffs, only the established LLOQ is listed.

	Positive control result		Nominal conc.	Lower limit	Upper limit	Within range	Comments
	Mean	%CV					
Morphine	0.473	3.31	0.48	0.310	0.650	y	
Dihydrocodeine	0.583	4.35	0.47	0.310	0.630	y	
Codeine	0.253	3.41	0.27	0.180	0.360	y	
Amphetamine	0.464	4.07	0.51	0.330	0.690	y	
Oxycodone	0.532	5.51	0.47	0.300	0.630	y	
6-acetyl morphine	0.841	2.68	0.57	0.370	0.770	n	* Beyond calibration range
MDA	0.394	6.58	0.42	0.270	0.570	y	
Methamphetamine	0.516	2.57	0.60	0.390	0.810	y	
MDMA	0.661	9.37	0.74	0.480	1.000	y	
MDEA	0.653	7.35	0.63	0.410	0.850	y	
Benzoyllecgonine	0.500	4.07	0.36	0.230	0.490	n	
Tramadol	0.434	2.18	0.52	0.340	0.700	y	
Cocaine	0.862	3.61	0.90	0.590	1.220	y	
Norbuprenorphine	0.091	9.17	0.06	0.039	0.081	n	
Cocaeethylene	0.876	3.80	0.58	0.380	0.780	n	* Beyond calibration range
Fentanyl	0.224	3.17	0.14	0.090	0.190	n	
Buprenorphine	0.065	4.78	0.05	0.033	0.068	y	
EDDP	0.546	4.17	0.41	0.270	0.550	y	
Methadone	0.866	8.91	0.58	0.380	0.780	n	
Lorazepam	0.198	3.18	0.27	0.180	0.360	y	
Alprazolam	0.255	4.23	0.23	0.150	0.310	y	
Nordiazepam	0.230	2.83	0.33	0.210	0.450	y	
Temazepam	0.177	3.27	0.25	0.160	0.340	y	
Diazepam	0.224	1.89	0.27	0.180	0.360	y	

Table 2. Results from external quality control (EQA) samples. 18/22 compounds were within the acceptable concentration ranges. The concentrations of 6-acetyl morphine and fentanyl were beyond the calibration range of this analytical method.

Conclusion

We have developed an optimized procedure for the analysis of a comprehensive drug panel in hair samples that meets the requirements of SoHT for sensitivity. The extraction was optimized to accommodate a wide variety of compounds including amine stimulants, natural and synthetic opioids, benzodiazepines and other common drugs of abuse. The Oasis MCX 96-well plates resulted in consistent recoveries and well controlled matrix effects. The chromatographic method was rapid, with all peaks eluting by 3.1 minutes while achieving baseline separation from potential interfering isomers. The Xevo TQ Absolute Triple Quadrupole Mass Spectrometer resulted in

quantitative results that were accurate and precise over the entire calibration range, meeting the SoHT sensitivity requirements for all the analytes, with only a couple of exceptions. External positive control samples confirmed the accuracy of the method with all compounds identified and >80% of compounds within the reference ranges. The combination of efficient sample preparation, rapid chromatography and accurate and precise quantification result in a method that can be used to accurately quantitate a variety of drugs in hair samples.

Appendix 1

Analyte	R.T.	Cone volt. (V)	Parent	MRM-1	CE-1	MRM-2	CE-2
Morphine	0.86	25	286.1	201.1	25	165.1	35
Oxymorphone	0.91	25	302.1	227.0	25	242.1	25
Hydromorphone	0.97	25	286.1	185.0	30	157.0	40
Dihydrocodeine	1.15	25	302.2	199.0	30	128.1	60
Naloxone	1.15	10	328.2	212.0	38	253.0	28
Codeine	1.17	25	300.2	215.1	25	165.1	40
Noroxycodone	1.25	12	302.2	187.1	26	227.1	30
Naltrexone	1.26	6	342.3	324.2	18	270.2	26
Amphetamine	1.28	25	136.1	119.0	10	91.0	10
Oxycodone	1.28	25	316.1	241.1	25	256.2	25
6-acetyl morphine	1.29	5	328.3	165.1	35	211.2	25
MDA	1.30	22	180.1	163.1	8	105.0	20
Metadesnitazine	1.37	25	338.4	100.2	25	121.1	25
Hydrocodone	1.34	6	300.3	199.1	28	171.1	36
O-desmethyl Tramadol	1.33	25	250.2	58.1	15	--	--
Methamphetamine	1.36	24	150.1	119.1	9	91.0	15
MDMA	1.37	26	194.1	163.0	10	105.0	22
Phentermine	1.43	24	150.0	133.1	9	91.0	15
MDEA	1.48	26	208.1	163.1	10	105.0	24
Ritalinic Acid	1.49	25	220.1	84.0	20	56.0	40
Norfentanyl	1.54	25	233.2	84.0	15	177.2	15
Benzoylcegonine	1.53	36	290.1	168.1	18	105.0	32
7-aminoclonazepam	1.53	50	286.1	121.0	30	222.1	26
Tramadol	1.68	25	264.2	58.1	15	--	--
N-desmethyl Tramadol	1.70	25	250.1	44.0	10	232.2	7
Methylphenidate	1.70	25	234.2	84.0	15	91.0	40
7-aminoflunitrazepam	1.71	34	284.1	135.0	26	226.9	22
Cocaine	1.81	42	304.2	182.2	34	82.1	20
Normeperidine	1.82	25	234.2	160.1	15	131.0	28
Meperidine	1.83	25	248.2	174.1	20	220.2	20
Norbuprenorphine	1.91	25	414.4	101.3	48	57.1	43
Chlordiazepoxide	1.94	34	300.0	283.0	12	227.0	20
Trazodone	1.99	25	372.2	176.1	20	148.0	35
Cocaethylene	2.01	42	318.2	196.2	20	105.0	38
Phencyclidine	2.08	25	244.2	86.1	12	159.1	12
N-Pyrrolidino Etonitazine	2.19	25	395.4	98.2	20	107.1	40
Fentanyl	2.14	25	337.2	188.1	22	105.0	35
α -hydroxymidazolam	2.13	2	342.1	168.1	40	203.1	24
Midazolam	2.17	16	326.1	223.1	36	291.1	24
Etonitazine	2.23	25	397.4	100.2	25	107.1	30
Flurazepam	2.23	40	388.2	315.1	26	100.1	28
Buprenorphine	2.27	5	468.4	55.1	50	101.2	40
EDDP	2.37	25	278.2	234.1	30	249.2	25
Methadone	2.58	25	310.2	265.2	15	105.0	25
α -hydroxylprazolam	2.55	50	325.1	297.1	25	243.1	30
α -hydroxytriazolam	2.55	28	359.1	176.1	24	141.0	38
Nitrazepam	2.56	50	282.1	236.1	20	180.1	36
Oxazepam	2.63	50	289.1	243.1	20	104.1	30
Lorazepam	2.70	50	323.0	277.0	20	229.1	30
Clonazepam	2.69	50	316.0	270.1	25	241.1	35
Alprazolam	2.72	50	309.1	205.1	40	281.1	26
2-hydroxyethyl Flurazepam	2.72	25	333.1	109.0	25	194.0	20
Nordiazepam	2.72	50	271.1	140.0	30	165.0	28
Triazolam	2.78	28	343.1	239.1	38	308.1	24
Desalkylflurazepam	2.82	25	289.1	140.0	30	226.1	25
Flunitrazepam	2.83	50	314.1	268.1	25	239.1	30
Temazepam	2.91	50	301.1	255.1	20	177.1	46
Diazepam	3.08	50	285.1	154.0	26	193.1	30

Appendix 1. Retention times (RT) cone voltages, precursor and product ions, and collision energies used for the compounds in this application.

Appendix 2

	Within batch statistics					
	Low		Medium		High	
	Mean	%CV	Mean	%CV	Mean	%CV
Morphine	101.3	4.2	105.1	5.8	93.4	5.6
Oxymorphone	98.6	2.7	100.4	1.1	96.4	3.3
Hydromorphone	98.2	2.6	101.5	1.2	97.3	4.2
Dihydrocodeine	98.1	2.5	101.5	1.8	97.2	4.8
Naloxone	91.5	5.1	100.8	4.5	94.2	4.4
Codeine	92.0	8.5	98.4	0.7	94.5	4.3
Noroxycodone	94.7	7.7	99.5	5.8	94.0	4.3
Amphetamine	117.6	10.9	101.5	2.5	95.8	2.1
Naltrexone	102.5	4.7	98.8	3.3	91.6	4.5
Oxycodone	96.4	2.5	103.6	1.9	97.4	3.6
6-acetyl morphine	93.3	5.4	103.1	5.6	94.8	2.4
MDA	99.2	10.0	102.7	3.3	96.4	5.3
Metadesnitazine	95.9	4.1	97.6	2.3	86.9	3.4
Hydrocodone	98.2	4.1	103.5	1.6	94.5	3.6
O-desmethyl Tramadol	96.8	4.1	103.1	0.8	96.2	3.5
Methamphetamine	96.5	3.0	103.7	3.5	94.6	5.7
MDMA	96.2	6.1	102.0	5.1	97.8	6.9
Phentermine	ND	ND	44.0	85.5	92.3	7.2
MDEA	96.7	8.0	101.8	3.8	97.8	4.6
Ritalinic acid	82.7	9.0	94.7	7.1	94.3	5.1
Norfentanyl	91.5	4.3	101.4	2.8	105.8	5.1
Benzoylcegonine	100.5	3.2	100.9	1.5	94.5	2.8
7-aminoclonazepam	100.8	3.0	97.5	2.8	92.0	2.7
Tramadol	97.8	1.5	103.2	2.4	98.3	2.6
N-desmethyltramadol	96.5	5.5	105.2	3.4	96.0	3.0
Methylphenidate	99.3	1.7	101.0	1.6	95.5	2.7
7-aminoflunitrazepam	96.4	4.2	100.9	1.8	95.3	3.1
Cocaine	99.7	3.2	101.3	2.3	96.0	4.2
Norperidine	97.2	4.1	102.4	1.6	96.7	3.2

	Within batch statistics					
	Low		Medium		High	
	Mean	%CV	Mean	%CV	Mean	%CV
Meperidine	97.4	2.7	101.7	1.1	95.2	3.9
Norbuprenorphine	102.8	7.7	97.3	4.3	97.6	3.1
Chlorazepoxide	99.9	4.1	113.9	0.6	102.3	2.4
Trazodone	105.2	2.5	105.2	2.2	99.3	3.6
Cocethyline	99.0	2.3	101.4	1.9	96.5	3.3
Phencyclidine	98.0	2.1	101.5	1.0	95.7	3.7
N-Pyrrolidino Etonitazine	98.6	3.7	100.1	2.9	90.5	3.2
Fentanyl	99.5	2.8	101.5	2.3	94.2	2.6
α-Hydroxymidazolam	106.7	7.9	105.8	3.2	93.6	3.3
Midazolam	94.6	4.3	102.0	1.7	96.6	1.9
Etonitazine	96.4	5.8	100.3	4.1	91.8	4.2
Flurazepam	98.6	3.6	103.5	2.5	99.8	2.1
Buprenorphine	96.6	6.5	97.4	4.8	93.4	4.3
EDDP	100.7	4.0	102.2	1.9	96.5	3.5
Methadone	99.3	3.9	103.7	2.1	97.3	2.9
α-Hydroxyalprazolam	92.9	9.1	101.7	2.6	97.1	2.1
α-Hydroxytriazolam	94.8	9.9	101.8	2.2	99.3	3.1
Nitrazepam	96.5	4.9	101.3	2.1	100.2	3.8
Oxazepam	103.7	11.2	107.6	6.0	94.1	5.0
Lorazepam	97.8	10.1	103.6	2.1	95.9	4.9
Clonazepam	104.6	5.4	106.0	4.4	93.3	3.3
Alprazolam	97.8	5.9	100.3	1.2	95.7	3.5
2-hydroxyethylflurazepam	101.8	8.5	102.6	7.3	96.7	4.0
Nordiazepam	98.7	2.7	101.6	2.8	96.5	4.0
Triazolam	102.5	3.4	103.0	3.9	94.1	2.2
Desalkylflurazepam	94.7	2.5	103.0	3.0	96.6	2.8
Flunitrazepam	93.9	1.7	101.6	2.1	95.2	3.1
Temazepam	96.0	4.0	101.6	2.3	97.2	0.9
Diazepam	96.0	2.1	98.5	2.3	96.2	2.6

Appendix 2. Within batch accuracy and precision data for all compounds.

All compounds met validation criteria except for phentermine and metadesnitazine, as mentioned previously. N=4 replicates.

Appendix 3

	Between batch statistics					
	Low		Medium		High	
	Mean	%CV	Mean	%CV	Mean	%CV
Morphine	104.1	3.9	103.7	3.4	102.9	6.6
Oxymorphone	102.6	3.0	102.7	1.7	102.7	5.0
Hydromorphone	102.7	3.1	102.6	1.8	102.9	6.4
Dihydrocodeine	103.0	4.7	101.8	4.7	102.7	5.3
Naloxone	103.0	6.6	99.8	4.5	99.8	7.2
Codaine	100.4	6.7	101.8	2.3	103.1	6.0
Norexycodone	102.4	5.2	100.9	3.4	103.4	6.8
Amphetamine	105.6	8.0	102.2	3.5	99.8	4.1
Naltrexone	103.6	3.2	104.1	3.0	102.9	7.3
Oxycodone	102.9	4.8	104.9	1.1	104.8	5.2
6-acetylmorphine	105.3	7.1	103.1	3.0	104.1	7.2
MDA	104.9	6.5	103.2	3.4	102.1	4.7
Metadesnitazine	110.7	11.3	104.2	12.3	92.4	16.9
Hydrocodone	105.5	4.7	103.8	1.8	102.3	6.3
O-desmethyl Tramadol	103.0	4.1	102.8	1.5	101.7	5.0
Methamphetamine	100.3	3.9	99.8	4.6	102.5	6.6
MDMA	100.4	4.0	99.3	5.4	107.0	13.3
Phentermine	99.5	19.6	91.1	32.3	97.2	9.4
MDEA	102.7	5.2	100.7	1.0	102.4	6.4
Ritalinic acid	102.6	11.4	95.8	4.9	105.0	7.5
Norfentanyl	99.6	6.0	101.1	4.0	106.1	5.7
Benzoylgonine	103.4	2.6	102.8	2.4	101.5	5.8
7-aminoclonazepam	102.9	5.3	101.5	3.4	101.6	6.7
Tramadol	103.6	3.8	103.8	2.2	103.4	4.5
N-desmethyiltramadol	102.5	4.8	101.2	2.4	104.5	9.2
Methylphenidate	104.1	3.6	101.9	1.6	101.9	5.6
7-aminoflunitrazepam	102.0	3.6	102.4	2.5	102.3	5.6
Cocaine	103.4	3.8	102.0	0.9	101.9	5.0
Norpiperidine	103.5	4.4	102.0	0.5	101.7	4.5

	Between batch statistics					
	Low		Medium		High	
	Mean	%CV	Mean	%CV	Mean	%CV
Meperidine	102.7	3.3	102.8	2.3	101.9	5.7
Norbuprenorphine	99.4	8.0	100.1	3.9	101.1	6.2
Chlorazepoxide	105.7	3.9	114.4	3.5	110.0	4.6
Trazodone	104.2	3.7	103.9	1.6	103.0	5.0
Cosarethylene	103.2	2.8	102.0	2.2	101.6	5.2
Phencyclidine	103.0	4.0	102.6	1.7	102.8	5.7
N-Pyrrolidino Etionitazine	105.8	11.0	100.8	12.7	96.3	11.4
Fentanyl	105.8	7.1	105.7	4.6	101.5	8.3
α-Hydroxymidazolam	103.3	4.5	103.9	6.4	97.6	5.8
Midazolam	102.4	4.8	104.1	2.6	101.8	3.9
Etionitazine	104.7	10.3	101.5	10.6	95.6	10.4
Flurazepam	103.2	3.0	105.4	3.0	105.6	5.1
Buprenorphine	104.0	5.4	99.6	4.0	100.6	6.6
EDDP	102.4	2.1	102.6	1.3	102.0	4.4
Methadone	103.3	3.2	102.4	2.2	103.1	4.6
α-Hydroxyalprazolam	103.5	6.0	102.1	2.0	103.8	6.4
α-Hydroxytriazolam	101.5	4.7	103.5	5.2	102.8	5.1
Nitrazepam	103.1	7.8	102.9	1.2	103.5	4.3
Oxazepam	104.2	2.5	101.5	4.7	101.6	5.2
Lorazepam	102.0	4.3	106.2	3.6	104.5	5.7
Clonazepam	102.8	4.7	106.2	4.6	104.0	6.5
Alprazolam	103.2	3.9	102.9	2.6	102.7	6.3
2-hydroxyethylflurazepam	103.8	3.1	103.4	3.3	102.6	6.0
Nordiazepam	102.5	3.1	102.7	1.4	102.4	4.6
Triazolam	103.3	2.1	103.3	1.3	102.6	5.7
Desalkylflurazepam	104.0	5.4	105.9	5.5	101.6	5.0
Flunitrazepam	102.6	6.2	102.8	3.3	102.1	5.5
Temazepam	102.1	4.2	101.1	1.3	102.1	4.9
Diazepam	104.1	4.9	102.4	3.1	101.7	6.1

Appendix 3. Between batch accuracy and precision data for all compounds. All compounds met validation criteria except for phentermine and metadesnitazine, as mentioned previously. N=5 batches.

References

1. G.A.A. Cooper, R. Kronstrand, P. Kintz. Society of Hair Testing Guidelines for Drug Testing in Hair. *Forensic Science International* 281 (2012) 20–24.
2. Statements of the Society of Hair Testing Concerning the Examination of Drugs in Human Hair [cited 14th Aug 2024]. Available from: <https://www.soht.org/statements> <<https://www.soht.org/>>
3. J. Hu, H. Chen, *et al.* Pulverization is a crucial step – A Comparative Study of Different Pretreatments in Hair Drug Testing. *Journal of Analytical Toxicology*, 47 (2023) 346–352.

Featured Products

ACQUITY UPLC I-Class PLUS System <

<https://www.waters.com/nextgen/global/products/chromatography/chromatography-systems/acquity-uplc-i-class-plus-system.html>>

Xevo TQ Absolute Triple Quadrupole Mass Spectrometer <

<https://www.waters.com/nextgen/global/products/mass-spectrometry/mass-spectrometry-systems/xevo-tq-absolute.html>>

MassLynx Mass Spectrometry Software <<https://www.waters.com/nextgen/global/products/informatics-and-software/mass-spectrometry-software/masslynx-mass-spectrometry-software.html>>

720008769, June 2025



© 2025 Waters Corporation. All Rights Reserved.

[이용 약관](#) [개인정보 보호정책](#) [상표](#) [채용정보](#) [법적 고지](#) 및 [개인정보 보호 고지](#) [쿠키](#) [쿠키 기본설정](#)