

## Application Note

# Temperature Control Using Waters LC Purification Systems with Timberline's Column and Mobile Phase Heaters: Optimizing Preparative Performance

---

Jinxia Xia, Jo-Ann M. Jablonski, Darcy Shave, Kathy Lawrence

Waters Corporation, United States

*Published on July 02, 2025*

## Application Brief

This is an Application Brief and does not contain a detailed Experimental section.

---

## Abstract

Temperature is a useful parameter for optimizing separations in both analytical and preparative chromatography. As the temperature rises, mobile phase viscosity and system pressure decrease, and the selectivity of the separation changes. Temperature also impacts retention times, compound resolution, sensitivity, and overall run time. The increased resolution can potentially allow one to load more sample onto the column. Precise control of the separation temperature is essential to achieving reproducible results.

## Benefits

- Minimizing method redevelopment at the prep scale improves process efficiency and reproducibility, ensuring

predictable and reliable outcomes for isolating small and large molecules, such as oligonucleotides and peptides.

- Elevated temperature reduces system backpressure and enables one to consider using of sub-5  $\mu\text{m}$  Waters™ preparative Optimum Bed Density (OBD™) columns to increase productivity through faster separations, increased loading capacity, lower solvent consumption, shorter fraction dry-down times, and reduced waste disposal costs.
- Enabling the substitution of acetonitrile with methanol provides a more environmentally sustainable and economically efficient purification process.

---

## Introduction

Although temperature control is widely implemented in analytical HPLC to improve separations and ensure consistent and reliable outcomes, temperature is seldom controlled or used as a parameter for manipulating chromatography at the preparative scale for two reasons. First, high flow rate separations occur at the temperature of the incoming solvent and efficient heating of the mobile phase entering the column is challenging at these high flow rates. Second, large diameter columns cannot be effectively heated from the outside simply by using insulation, heated blankets or ovens. Ideally, analytical separations developed with temperature control should be scaled to prep at the same temperature to eliminate variability in the chromatography which can make the target identification and isolation ambiguous or lead to product loss.

When used with the Waters AutoPurification System, Timberline's column and mobile phase heaters provide precise and consistent temperature control for preparative separations, allowing easier scale-up from UPLC/UHPLC to preparative methods. This integrated approach minimizes the need for method redevelopment, improves reproducibility, enhances hydrophobic compound solubility and boosts operational efficiency, which is particularly valuable in small molecule isolations and biological applications such as oligonucleotide and peptide purification. Temperature control also enhances flexibility in purification workflows, supporting green chemistry initiatives by enabling the substitution of acetonitrile with methanol. Elevated temperature reduces system backpressure, allowing the usage of sub-5  $\mu\text{m}$  particles in larger-dimension preparative columns (*e.g.*, 10 mm ID), which may increase loading capacity, minimize run-times, reduce solvent consumption, shorten dry-down times and lower waste disposal costs. This technical brief illustrates that comparable purification results can be achieved using methanol with sub-5  $\mu\text{m}$  10 mm ID columns, an approach that is both environmentally

sustainable and economically viable. It also illustrates the precision and stability of temperature control across various flow rates and mobile phase compositions, showcasing the reliability of this solution.



Waters AutoPurification System with PDA and ACQUITY QDa II Detectors




Timberline TL-105 D Column Oven (two temperature-controlled zones, one for the column oven and the other for the internal mobile phase heater with active heating)

*Figure 1. Waters AutoPurification System and Timberline TL-105 D Column Oven.*

## Results and Discussion

### Temperature control impact on separation

Methanol usually results in longer retention time than acetonitrile in reversed-phase. Figure 2 illustrates that for both solvents, the compounds eluted earlier when the temperature was increased to 60 °C from ambient conditions.

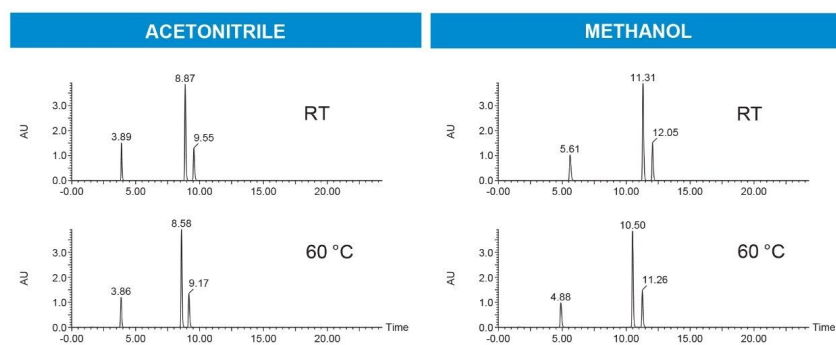

*Figure 2. Gradient separations using aqueous/organic mobile phases at room temperature and at 60 °C on a 10 x 100 mm, 3.5 µm XBridge™ Premier BEH™ C<sub>18</sub> OBD Preparative Column; 2.4 mg; 254 nm.*

## Elevated temperature reduces system backpressure for productivity improvements

While temperature is a useful parameter for optimizing separations, it also reduces system and column backpressure, enabling the use of columns with smaller particle stationary phases. Small particle packings increase column efficiency and may enhance target compound peak areas and sensitivity. Reduced peak widths resulting from columns packed with small particles also produce smaller fraction volumes, ultimately decreasing fraction drying times. These factors all contribute to increasing overall operational efficiency and lowering processing costs. Figure 3 illustrates scaling the separation from UHPLC to the preparative scale using a 3.5 µm, 10 mm ID prep column. Figure 4 shows the separation on the 19 x 50 mm prep column at 24 mL/min at 60 °C.

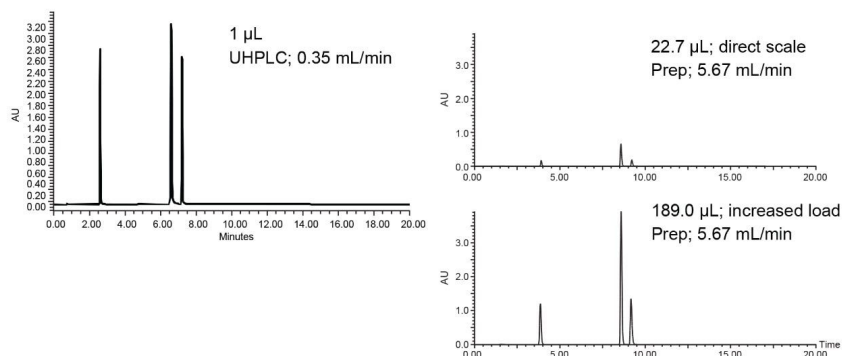


Figure 3. Scaling from UHPLC on a 2.1 x 100 mm, 3.5 µm XBridge Premier BEH C<sub>18</sub> Column to prep on a 10 x 100 mm, 3.5 µm XBridge Premier BEH C<sub>18</sub> OBD Preparative Column. All separations were performed using acetonitrile at 60 °C. Top right: Direct scaling from UHPLC (1 µL, 12.6 µg) to Prep (22.7 µL, 286.7 µg). Bottom right: Increased load (189 µL, 2.4 mg).


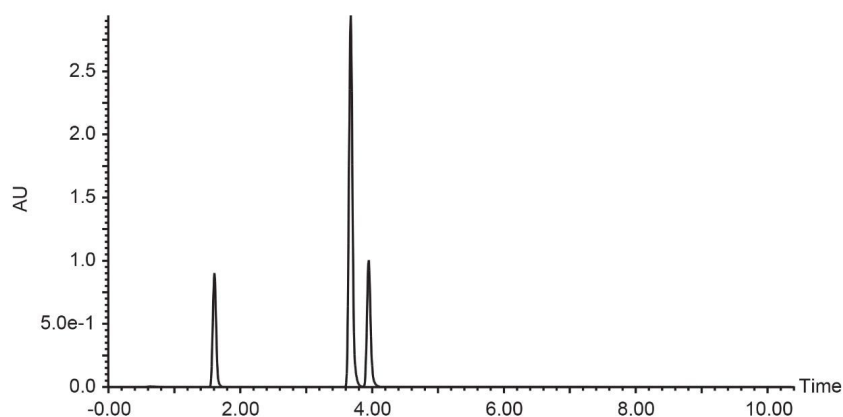


Figure 4. Scaled HPLC separation on a 19 x 50 mm, 5 µm XBridge BEH C<sub>18</sub> OBD Preparative Column using acetonitrile at 60 °C. The injection volume was 341.2 µL (4.3 mg); 254 nm.

## Enable the use of greener solvents as alternatives to acetonitrile

Acetonitrile is often used in purification laboratories as its low viscosity promotes low backpressure even at the

high flow rates used in prep chromatography. However, preparative chromatography consumes large amounts of solvents, which has an environmental impact. With the growing trend of green chemistry, more purification labs are evaluating alternative, more environmentally-friendly solvents. Figure 5 illustrates the compound separation using methanol at 24 mL/min.

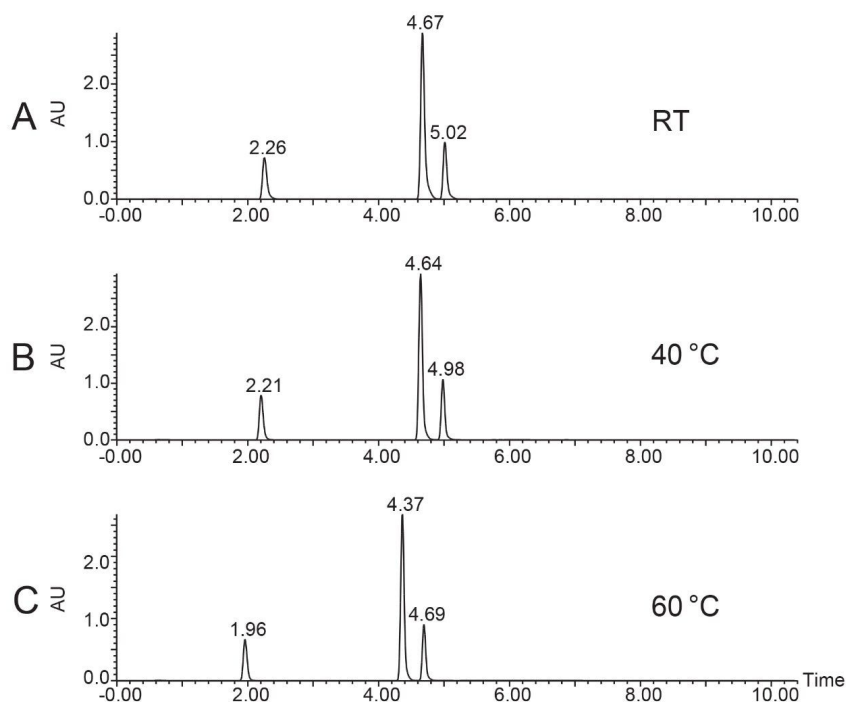

*Figure 5. Separations using methanol at room temperature, 40 °C and at 60 °C on a 19 x 50 mm, 5  $\mu$ m XBridge BEH C<sub>18</sub> OBD Preparative Column; 4.3 mg; 254 nm.*

## Provides stable/controlled heating for consistency in separations

Precision and stability evaluation of the temperature control and system performance at different flow rates and temperatures is shown in Figures 6–9. The results show minimal temperature variation over the course of the chromatographic runs. As expected, increased temperature reduces the system/column back pressure. The temperature and pressure data collected over the course of preparative chromatographic runs also illustrate the reliability of the Timberline oven when configured in the AutoPurification System.

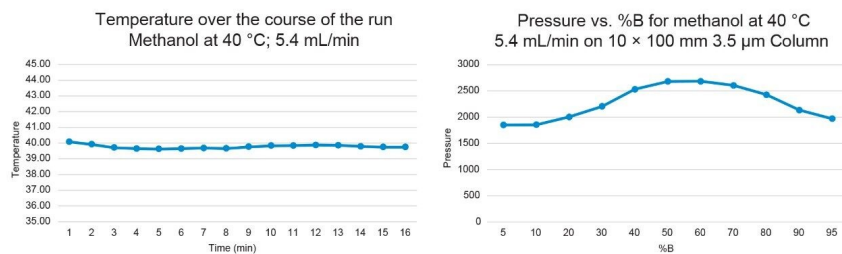


Figure 6. Temperature and pressure profiles over the course of the chromatographic run on the 3.5 μm, 10 x 100 mm column @ 40 °C.

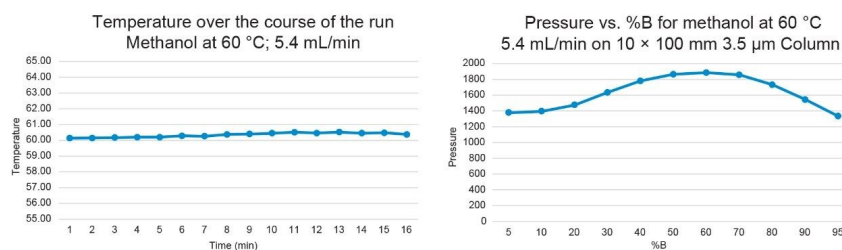


Figure 7. Temperature and pressure profiles over the course of the chromatographic run on the 3.5 μm, 10 x 100 mm column @ 60 °C.

Figures 6–7 demonstrate that the temperature remained highly stable at 5.4 mL/min flow rate, fluctuating by less than 0.5 °C at 40 °C and 60 °C throughout the runs.

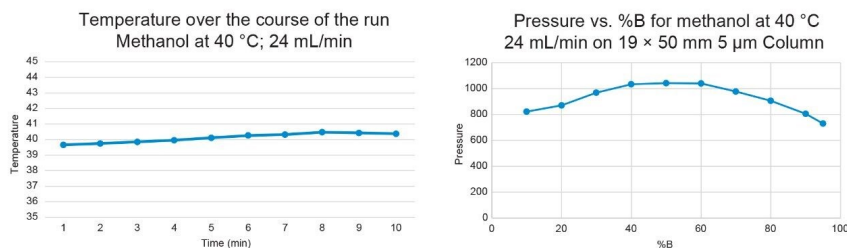


Figure 8. Temperature and pressure profiles over the course of the chromatographic run on the 5 µm, 19 x 50 mm column @ 40 °C.

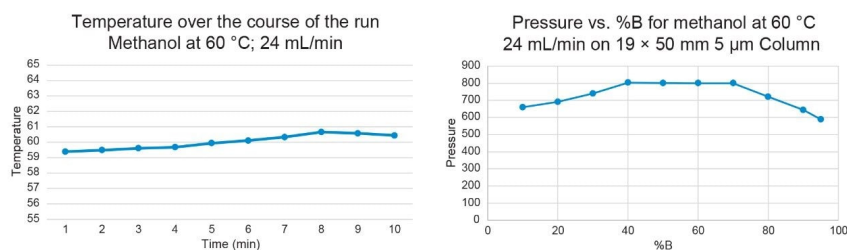


Figure 9. Temperature and pressure profiles over the course of the chromatographic run on the 5 µm, 19 x 50 mm column @ 60 °C.

Figures 8–9 demonstrate that the temperature remained highly stable at the 24 mL/min flow rate, fluctuating by less than 1°C at 40 °C and 60 °C throughout the run.

## Conclusion

Timberline's TL-105 D column oven configured with the Waters AutoPurification System provides precise and consistent temperature control when scaling from analytical to preparative methods. This significantly reduces the need for method redevelopment at the prep scale, enhances chromatographic efficiency and reproducibility and delivers predictable and reliable outcomes for various applications including small and large molecules such as oligonucleotides and peptides isolations.



This combined solution supports the growing demand for green chemistry by enabling the substitution of acetonitrile with methanol. Enhanced temperature control also lowers system backpressure, allowing the use of smaller particle size, larger dimension Waters preparative OBD columns. This results in faster separations, increased loading capacity, reduced solvent consumption, shorter fraction dry-down times, and lower waste disposal costs. These benefits contribute to a more environmentally sustainable and economically efficient purification process.

---

## References

1. Robert S. Plumb, Jeffrey R. Mazzeo. The Effect of Elevated Column Operating Temperatures on Chromatographic Performance. Waters Application Note. [720001799 <https://www.waters.com/nextgen/global/library/application-notes/2006/the-effect-of-elevated-column-operating-temperatures-on-chromatographic-performance.html>](https://www.waters.com/nextgen/global/library/application-notes/2006/the-effect-of-elevated-column-operating-temperatures-on-chromatographic-performance.html) . Accessed: June, 2006.

---

## Featured Products

LC Prep AutoPurification System <

<https://www.waters.com/nextgen/global/products/chromatography/chromatography-systems/lc-prep-autopurification-system.html>>

Modular Systems <<https://www.waters.com/nextgen/global/products/chromatography/chromatography-systems/modular-systems.html>>

LC Prep 150 System <<https://www.waters.com/nextgen/global/products/chromatography/chromatography-systems/lc-prep-150-system.html>>

MassLynx Mass Spectrometry Software <<https://www.waters.com/nextgen/global/products/informatics-and-software/mass-spectrometry-software/masslynx-mass-spectrometry-software.html>>

MaxPeak Premier OBD Preparative Columns <

<https://www.waters.com/nextgen/global/products/columns/maxpeak-premier-obd-preparative-columns.html>>

XBridge Premier Columns <<https://www.waters.com/nextgen/global/products/columns/xbridge-premier>>

[columns.html](#)>

720008874, June 2025



© 2025 Waters Corporation. All Rights Reserved.

[Terms of Use](#) [Privacy Notice](#) [Trademarks](#) [Careers](#) [Legal and Privacy Notices](#) [Cookies](#)  
[Cookie Preferences](#)