

Note d'application

## Separation of a GLP-1 Receptor Agonist and Structurally Similar Impurities Using BioResolve™ Peptide Phenyl-Hexyl+ and C<sub>18</sub>+ Columns

---

Hua Yang, Steve Shiner

Waters Corporation, United States

*Published on July 01, 2026*

### Application Brief

This is an Application Brief and does not contain a detailed Experimental section.

---

### Abstract

To demonstrate the use of BioResolve Peptide Phenyl-Hexyl+ and BioResolve Peptide C<sub>18</sub>+ reversed-phase (RP) Columns for separation of tirzepatide, a glucagon-like peptide-1 (GLP-1) receptor agonist, and its impurities.

---

### Introduction

GLP-1 therapeutics represent one of the fastest growing classes of biopharmaceuticals on the market. As these peptide-based drugs advance through development, manufacturing, and storage, it is critical to separate and

characterize their impurities to ensure product safety, stability, and efficacy.

Structurally similar peptide impurities such as deamidation, isoaspartate, single amino acid D- enantiomer and single amino acid substitution are particularly challenging to separate. This application brief shows that BioResolve Peptide Phenyl-Hexyl+ and BioResolve Peptide C<sub>18</sub>+ RP Columns can separate structurally similar impurities from tirzepatide, and that selectivity of these impurities can be modulated with appropriate selection of column chemistry.

---

## Results and Discussion

### The Solution

Waters BioResolve Peptide Phenyl-Hexyl+ and BioResolve Peptide C<sub>18</sub>+ RP Columns are specifically tuned for the separation of larger peptides and their impurities. These columns incorporate superficially porous particles with an average pore size of 230 Å, providing improved accessibility and chromatographic efficiency for molecules such as GLP-1 receptor agonists and insulins. Additionally, a controlled level of positive charge is applied to the particle surface which has been proven to improve peak shape and loading capacity of basic analytes, especially when using formic acid modified mobile phases.<sup>1</sup> Finally, the columns are built with MaxPeak™ Premier inert hardware designed to minimize non-specific adsorption (NSA) between the column hardware and the analytes, thereby improving recovery, consistency, and analytical robustness.<sup>2</sup>

BioResolve Peptide Phenyl-Hexyl+ and BioResolve Peptide C<sub>18</sub>+ RP Columns were used to separate a sample containing tirzepatide and seven known impurities (Figure 1). Both columns resolve D-Ser32 (Impurity 7) from the main peak, demonstrating that BioResolve Peptide RP Columns can be used to effectively separate challenging D-amino acid isomeric impurities of large peptides such as GLP-1s. Moreover, the elution order for the three deamidation species (Impurities 1, 2, and 3) is different on the two column chemistries (Phenyl-Hexyl+ vs. C<sub>18</sub>+). The Phenyl-Hexyl Column resolves Impurity 3 from Impurities 1 and 2, whereas the C<sub>18</sub>+ Column resolves Impurity 2 from Impurities 1 and 3. These differences in elution behavior highlight the complementary selectivity provided by these two unique stationary phases.

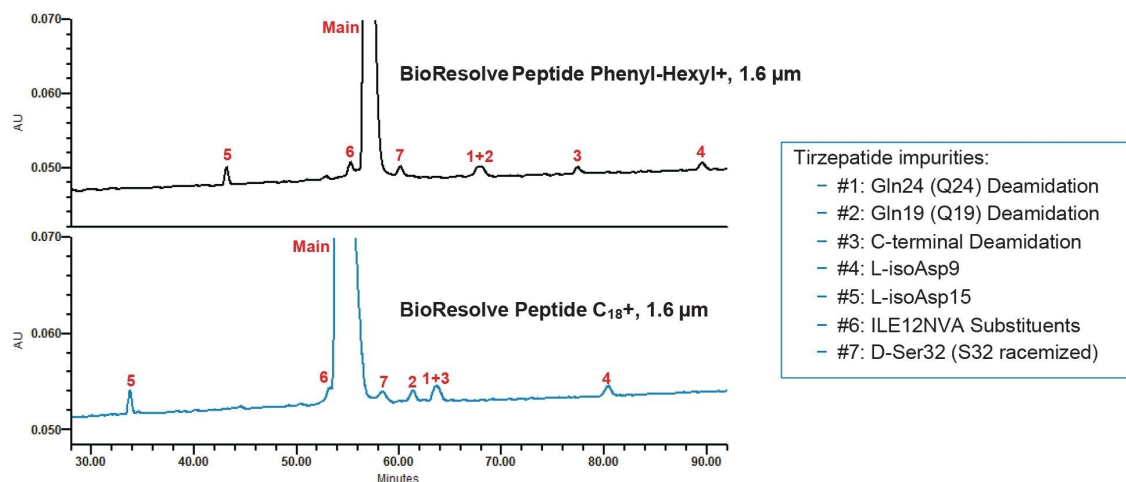


Figure 1. Separation of tirzepatide and seven spiked-in impurities (listed on the right) on a BioResolve Peptide Phenyl-Hexyl+ Column (top) and a BioResolve Peptide C<sub>18</sub>+ Column (bottom), both 1.6 μm in particle size and 2.1 x 150 mm in column dimensions. The two column chemistries provide different selectivity. Mobile phase A: 0.1% formic acid in water; mobile phase B: 0.1% formic acid in acetonitrile. Gradient on top: 32-36%B in 90 minutes; gradient at bottom: 37-41%B in 90 minutes. Flow rate: 0.3 mL/min. Column temperature: 50 °C. UV detection: 214 nm.

Even with a shallow gradient, separating some structurally similar impurities on the 2.1 x 150 mm columns remains difficult. Impurity 6 (Isoleucine→Norvaline) was not fully resolved from the main peak, and the three deamidation species were not baseline-separated, underscoring the inherent challenge of resolving closely related peptide variants (Figure 1). Other approaches such as increasing column length can further improve resolution.

Figure 2 shows the separation of tirzepatide and its impurities on a 2.1 x 150 mm (top) and a 2.1 x 300 mm (bottom) BioResolve Peptide Phenyl-Hexyl+ 1.6 μm Column. With the same run time, the 300 mm column can partially separate Impurity 1 and 2. A longer gradient time with a shallower gradient slope could be used to further improve resolution between Impurity 1 and 2. In addition, resolution of the two species eluting immediately before and after the main peak (Impurity 6 and 7) is improved on the 300 mm column compared to the 150 mm column. This suggests that longer columns may have more impact on the separation than running longer gradients on a shorter column, which has been observed in other separations.<sup>3</sup>

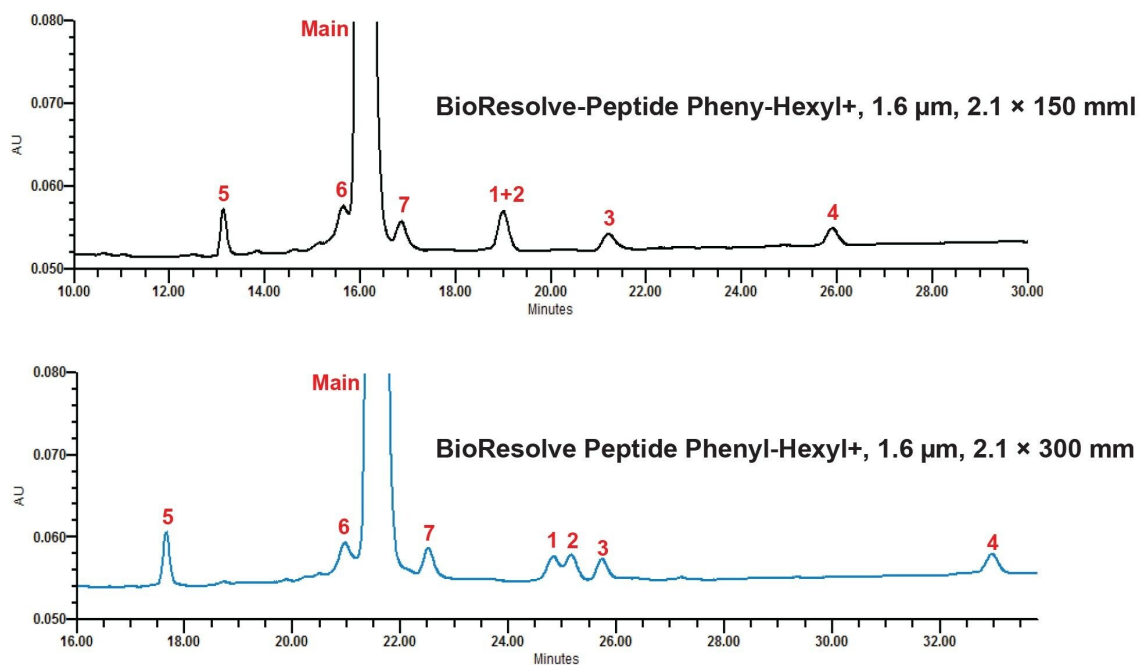


Figure 2. Separation of tirzepatide and seven spiked-in impurities on a 2.1 × 150 mm 1.6 μm BioResolve Peptide Phenyl-Hexyl+ Column (top) and a 2.1 × 300 mm 1.6 μm BioResolve Peptide Phenyl-Hexyl+ Column (bottom). The 300 mm column provides improved resolution compared to the 150 mm column with the same gradient time. Mobile phase A: 0.1% formic acid in water; mobile phase B: 0.1% formic acid in acetonitrile. Gradient on top: 35-39%B in 30 minutes; gradient at bottom: 36-40%B in 30 minutes. Flow rate: 0.3 mL/min. Column temperature: 50 °C. UV detection: 214 nm. The pressure for the 150 mm and the 300 mm column is ~6,320 psi and ~12,150 psi, excluding the system pressure.

## Conclusion

BioResolve Peptide Phenyl-Hexyl+ and BioResolve Peptide C<sub>18</sub>+ RP Columns are able to separate tirzepatide, a GLP-1 drug, from structurally similar impurities. The two different column chemistries (Phenyl-Hexyl+ and C<sub>18</sub>+) provide different selectivity, which can be useful depending on the separation needs. In addition, with the same run time, the 300 mm length column provides higher resolution than the 150 mm length column, even though the

gradient slope is 2x steeper for the 300 mm length column.

---

## References

1. Lauber M.A.; Koza S.M.; Fountain K.J. Increasing Peak Capacity in Reversed-Phase Peptide Separations with Charged Surface Hybrid (CSH) C<sub>18</sub> Columns. Waters Application Note. [720004568](#), 2013.
  2. Improving Chromatographic Separations of Biopharmaceuticals with MaxPeak High Performance Surfaces (HPS) Technology. Waters eBook. [720008110](#) <<https://www.waters.com/nextgen/global/library/library-details.html?documentid=720008110>> , 2024.
  3. Yang H.; Warren B.; Koza S. Development of Monoclonal Antibody Charge Variant Analysis Methods Using a BioResolve SCX mAb Column. Waters Application Note. [720006477](#), 2019.
- 

## Featured Products

[BioResolve Premier Columns <https://www.waters.com/nextgen/global/products/columns/bioresolve-premier-columns.html>](https://www.waters.com/nextgen/global/products/columns/bioresolve-premier-columns.html)

[MaxPeak Premier Columns <https://www.waters.com/nextgen/global/products/columns/maxpeak-premier-columns.html>](https://www.waters.com/nextgen/global/products/columns/maxpeak-premier-columns.html)

720009465, July 2026



© 2026 Waters Corporation. All Rights Reserved.

[Conditions d'utilisation](#) [Déclaration de confidentialité](#) [Marques](#) [Carrières](#) [Mentions légales](#)

---

et déclaration de confidentialité Cookies Préférences de cookies Ne vendez pas mes informations personnelles